



EA Engineering, Science,
and Technology, Inc.

South Central Region
405 S. Highway 121, Suite C-100
Lewisville, TX 75067
Telephone: 972-315-3922
Fax: 972-315-5181
www.eaest.com

13 March 2009

Mr. Gary Miller
Task Order Monitor
U.S. Environmental Protection Agency (EPA)
1445 Ross Avenue, Suite 1200
Dallas, TX 75202-2733

**Subject: Data Validation Report and Data Package (SDG ASA0086)
Phase 5 Ground Water Investigation
Ground Water Split Sampling (13 January 2009)
Gulfco Marine Maintenance Site RI/FS Oversight
U.S. Environmental Protection Agency Region 6
Remedial Action Contract 2, Contract: EP-W-06-004
Task Order: 0006-RICO-06JZ**

RECEIVED
2009 MAR 17 PM 1:16
SUPERFUND DIV.
REMEDIAL BRANCH
(6SF:R)

Dear Mr. Miller:

EA Engineering, Science, and Technology, Inc. (EA) is submitting one copy of the data validation report (Enclosure 2) and analytical data package (Enclosure 3) associated with the split ground water samples collected from monitoring wells NEMW32C and OCPT5 on 13 January 2009, and analyzed for volatile organic compounds (SW-846 Method 8260B). The attached table (Enclosure 1) compares the analytical results to the Preliminary Screening Values for Class 3 ground water (Table 18 of the remedial investigation/feasibility study) Work Plan, dated 16 May 2005 [Pastor, Behling & Wheeler, LLC]).

On 24 February 2009, EA transmitted the electronic version of the analytical data summary (in PDF format) via e-mail.

If you have any questions regarding this submittal, please call me at (972) 459-5040.

Sincerely,

Mark Paddack
Project Manager

Enclosures (3)



Mr. Gary Miller
13 March 2009
Page 2

cc: Michael Pheeny, EPA Contracting Officer (letter only)
Rena McClurg, EPA Project Officer (letter only)
Fritz Meyer, EA Program Manager (letter only via e-mail)
Jeff Hills, EA Financial Manager (letter only via e-mail)
File

Enclosure 1

Comparison of Ground Water Data and Preliminary Screening Values

GULFCO GROUND WATER SPLIT SAMPLE DATA - 13 JANUARY 2009
(LAB SDG ASA0086)

Sample ID	Lab Sample No.	Matrix	Collected	Volatile Organic Analyte	Result	Flag	Preliminary Screening Value ¹	Reporting Limit	Method Detection Limit	Units	Method	Dilution	Received	Analyzed
NEMW32C	1	WATER	1/13/2009	1,1,1,2-Tetrachloroethane	ND		7,860	1.00	0.332	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,1,1-Trichloroethane	0.761	J	20,000	1.00	0.360	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,1,2,2-Tetrachloroethane	ND		1,020	1.00	0.310	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,1,2-Trichloro-1,2,2-trifluoroethane	ND		NA	1.00	0.382	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,1,2-Trichloroethane	ND		500	1.00	0.352	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,1-Dichloroethane	22.7		730,000	1.00	0.374	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,1-Dichloroethene	1.46		700	1.00	0.427	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,1-Dichloropropene	ND		2,040	1.00	0.348	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,2,3-Trichloropropane	5.35		29.2	1.00	0.304	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,2,4-Trichlorobenzene	ND		7,000	1.00	0.484	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,2,4-Trimethylbenzene	ND		365,000	1.00	0.598	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,2-Dibromo-3-chloropropane (DBCP)	ND		20	5.00	0.342	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,2-Dibromoethane (EDB)	ND		5	1.00	0.298	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,2-Dichlorobenzene	ND		60,000	1.00	0.434	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,2-Dichloroethane	0.581	J	500	1.00	0.392	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,2-Dichloroethene (total)	114		NA	4.00	1.46	µg/L	8260B	2.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,2-Dichloropropane	ND		500	1.00	0.373	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,3,5-Trimethylbenzene	ND		365,000	1.00	0.488	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,3-Dichlorobenzene	ND		219,000	1.00	0.386	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,3-Dichloropropane	ND		2,040	1.00	0.292	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	1,4-Dichlorobenzene	ND		7,500	1.00	0.376	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	2,2-Dichloropropane	ND		3,010	1.00	0.390	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	2-Butanone (MEK)	ND		4,380,000	5.00	0.841	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	2-Chloroethyl vinyl ether	ND		186	5.00	0.623	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	2-Chlorotoluene	ND		146,000	1.00	0.395	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	2-Hexanone	ND		438,000	5.00	0.266	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	4-Chlorotoluene	ND		146,000	1.00	0.344	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	4-Methyl-2-pentanone (MIBK)	ND		584,000	5.00	0.416	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Acetone	0.978	J	6,570,000	5.00	0.819	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Acrolein	ND		3,650	10.0	1.29	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Acrylonitrile	ND		379	10.0	1.49	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Benzene	1.53		500	1.00	0.392	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Bromobenzene	ND		146,000	1.00	0.394	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Bromodichloromethane	ND		3,300	1.00	0.369	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Bromoform	ND		25,900	2.00	0.269	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Bromomethane	ND		10,200	2.00	0.723	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Carbon disulfide	1.14		730,000	1.00	0.383	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Carbon tetrachloride	ND		500	1.00	0.407	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Chlorobenzene	ND		10,000	1.00	0.333	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Chloroethane	ND		2,920,000	2.00	0.449	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Chloroform	ND		73,000	1.00	0.349	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Chloromethane	ND		15,700	2.00	0.482	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	cis-1,2-Dichloroethene	114		7,000	2.00	0.735	µg/L	8260B	2.00	1/14/2009	1/26/2009

GULFCO GROUND WATER SPLIT SAMPLE DATA - 13 JANUARY 2009
(LAB SDG ASA0086)

Sample ID	Lab Sample No.	Matrix	Collected	Volatile Organic Analyte	Result	Flag	Preliminary Screening Value ¹	Reporting Limit	Method Detection Limit	Units	Method	Dilution	Received	Analyzed
NEMW32C	1	WATER	1/13/2009	cis-1,3-Dichloropropene	ND		379	1.00	0.307	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Dibromochloromethane	ND		2,430	1.00	0.278	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Dibromomethane	ND		27,300	1.00	0.407	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Dichlorodifluoromethane	ND		1,460,000	2.00	0.518	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Ethylbenzene	ND		70,000	1.00	0.416	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Hexachlorobutadiene	ND		1,460	1.00	0.567	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Iodomethane	ND		NA	1.00	0.59	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Isopropylbenzene	ND		730,000	1.00	0.418	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Methyl acetate	ND		7,300,000	5.00	0.962	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Methyl tert-butyl ether (MTBE)	ND		73,000	1.00	0.336	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Methylcyclohexane	ND		36,500,000	5.00	0.723	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Methylene chloride	ND		500	1.00	0.422	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	n-Butanol	ND		NA	250	13.0	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	n-Butylbenzene	ND		292,000	1.00	0.878	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	n-Propylbenzene	ND		292,000	1.00	0.441	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	p-Isopropyltoluene	ND		NA	1.00	0.633	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	sec-Butylbenzene	ND		292,000	1.00	0.609	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Styrene	ND		10,000	1.00	0.310	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	tert-Butylbenzene	ND		292,000	1.00	0.450	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Tetrachloroethene	0.519	J	500	1.00	0.398	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Toluene	0.771	J	100,000	1.00	0.391	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	trans-1,2-Dichloroethene	0.531	J	10,000	1.00	0.372	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	trans-1,3-Dichloropropene	ND		2,040	1.00	0.209	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	trans-1,4-Dichloro-2-butene	ND		NA	5.00	0.357	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Trichloroethene	36.0		500	1.00	0.449	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Trichlorofluoromethane	ND		2,190,000	2.00	0.474	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Vinyl acetate	ND		7,300,000	2.00	0.293	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Vinyl chloride	ND		200	2.00	0.402	µg/L	8260B	1.00	1/14/2009	1/26/2009
NEMW32C	1	WATER	1/13/2009	Xylenes (total)	ND		1,000,000	3.00	1.20	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,1,1,2-Tetrachloroethane	ND		7,860	1.00	0.332	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,1,1-Trichloroethane	ND		20,000	1.00	0.360	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,1,2,2-Tetrachloroethane	ND		1,020	1.00	0.310	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,1,2-Trichloro-1,2,2-trifluoroethane	ND		NA	1.00	0.382	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,1,2-Trichloroethane	ND		500	1.00	0.352	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,1-Dichloroethane	ND		730,000	1.00	0.374	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,1-Dichloroethene	ND		700	1.00	0.427	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,1-Dichloropropene	ND		2,040	1.00	0.348	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,2,3-Trichloropropane	ND		29.2	1.00	0.304	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,2,4-Trichlorobenzene	ND		7,000	1.00	0.484	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,2,4-Trimethylbenzene	ND		365,000	1.00	0.598	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,2-Dibromo-3-chloropropane (DBCP)	ND		20	5.00	0.342	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,2-Dibromoethane (EDB)	ND		5	1.00	0.298	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	1,2-Dichlorobenzene	ND		60,000	1.00	0.434	µg/L	8260B	1.00	1/14/2009	1/26/2009

GULFCO GROUND WATER SPLIT SAMPLE DATA - 13 JANUARY 2009
(LAB SDG ASA0086)

Sample ID	Lab Sample No.	Matrix	Collected	Volatile Organic Analyte	Result	Flag	Preliminary Screening Value ¹	Reporting Limit	Method Detection Limit	Units	Method	Dilution	Received	Analyzed
OCPTS	2	WATER	1/13/2009	1,2-Dichloroethane	ND		500	1.00	0.392	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	1,2-Dichloroethene (total)	ND		NA	2.00	0.730	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	1,2-Dichloropropane	ND		500	1.00	0.373	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	1,3,5-Trimethylbenzene	ND		365,000	1.00	0.488	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	1,3-Dichlorobenzene	ND		219,000	1.00	0.386	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	1,3-Dichloropropane	ND		2,040	1.00	0.292	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	1,4-Dichlorobenzene	ND		7,500	1.00	0.376	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	2,2-Dichloropropane	ND		3,010	1.00	0.390	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	2-Butanone (MEK)	ND		4,380,000	5.00	0.841	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	2-Chloroethyl vinyl ether	ND		186	5.00	0.623	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	2-Chlorotoluene	ND		146,000	1.00	0.395	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	2-Hexanone	ND		438,000	5.00	0.266	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	4-Chlorotoluene	ND		146,000	1.00	0.344	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	4-Methyl-2-pentanone (MIBK)	ND		584,000	5.00	0.416	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Acetone	2.31	J	6,570,000	5.00	0.819	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Acrolein	ND		3,650	10.0	1.29	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Acrylonitrile	ND		379	10.0	1.49	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Benzene	ND		500	1.00	0.392	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Bromobenzene	ND		146,000	1.00	0.394	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Bromodichloromethane	ND		3,300	1.00	0.369	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Bromoform	ND		25,900	2.00	0.269	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Bromomethane	ND		10,200	2.00	0.723	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Carbon disulfide	0.614	J	730,000	1.00	0.383	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Carbon tetrachloride	ND		500	1.00	0.407	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Chlorobenzene	ND		10,000	1.00	0.333	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Chloroethane	ND		2,920,000	2.00	0.449	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Chloroform	ND		73,000	1.00	0.349	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Chloromethane	ND		15,700	2.00	0.482	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	cis-1,2-Dichloroethene	ND		7,000	1.00	0.367	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	cis-1,3-Dichloropropene	ND		379	1.00	0.307	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Dibromochloromethane	ND		2,430	1.00	0.278	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Dibromomethane	ND		27,300	1.00	0.407	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Dichlorodifluoromethane	ND		1,460,000	2.00	0.518	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Ethylbenzene	ND		70,000	1.00	0.416	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Hexachlorobutadiene	ND		1,460	1.00	0.567	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Iodomethane	ND		NA	1.00	0.590	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Isopropylbenzene	ND		730,000	1.00	0.418	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Methyl acetate	ND		7,300,000	5.00	0.962	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Methyl tert-butyl ether (MTBE)	ND		73,000	1.00	0.336	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Methylcyclohexane	ND		36,500,000	5.00	0.723	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	Methylene chloride	ND		500	1.00	0.422	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	n-Butanol	ND		NA	250	13.0	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPTS	2	WATER	1/13/2009	n-Butylbenzene	ND		292,000	1.00	0.878	µg/L	8260B	1.00	1/14/2009	1/26/2009

GULFCO GROUND WATER SPLIT SAMPLE DATA - 13 JANUARY 2009
(LAB SDG ASA0086)

Sample ID	Lab Sample No.	Matrix	Collected	Volatile Organic Analyte	Result	Flag	Preliminary Screening Value ¹	Reporting Limit	Method Detection Limit	Units	Method	Dilution	Received	Analyzed
OCPT5	2	WATER	1/13/2009	n-Propylbenzene	ND		292,000	1.00	0.441	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	p-Isopropyltoluene	ND		NA	1.00	0.633	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	sec-Butylbenzene	ND		292,000	1.00	0.609	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	Styrene	ND		10,000	1.00	0.310	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	tert-Butylbenzene	ND		292,000	1.00	0.450	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	Tetrachloroethene	ND		500	1.00	0.398	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	Toluene	ND		100,000	1.00	0.391	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	trans-1,2-Dichloroethene	ND		10,000	1.00	0.372	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	trans-1,3-Dichloropropene	ND		2,040	1.00	0.209	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	trans-1,4-Dichloro-2-butene	ND		NA	5.00	0.357	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	Trichloroethene	ND		500	1.00	0.449	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	Trichlorofluoromethane	ND		2,190,000	2.00	0.474	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	Vinyl acetate	ND		7,300,000	2.00	0.293	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	Vinyl chloride	ND		200	2.00	0.402	µg/L	8260B	1.00	1/14/2009	1/26/2009
OCPT5	2	WATER	1/13/2009	Xylenes (total)	ND		1,000,000	3.00	1.20	µg/L	8260B	1.00	1/14/2009	1/26/2009

Notes:

- 7,300** Indicates an exceedance of the preliminary screening value for Class 3 ground water
- ¹ Preliminary screening values for Class 3 ground water from Table 18 (human health risk values) of the Remedial Investigation/Feasibility Study Work Plan, dated 16 May 2005 (Pastor, Behling, Wheeler, LLC)
- J Estimated value; result is less than the reporting limit.
- ND Not detected
- NA Not applicable
- µg/L Microgram per liter

Enclosure 2

Data Validation Report

DATA VALIDATION REPORT

Site Name: Gulfco Marine Maintenance Site
Freeport, Brazoria County, Texas

Laboratory: Test America, Inc. – Austin, TX

QA Reviewer: Kim Wallace-Wymore, EA Engineering, Science, and
Technology, Inc. (EA), Dallas, TX

SDG No.: ASA0086

Sample Nos.: NEMW32C, OCPT5, TRIP BLANK

Matrix: Ground Water

QC Criteria Reviewed: Review criteria listed in Section 2.0 was performed for all above
samples.

Report Date: 3 February 2009

1.0 INTRODUCTION

Data were validated according to U.S. Environmental Protection Agency (EPA) documents “National Functional Guidelines for Organic Data Review” (EPA 2008). In addition, the site-specific Sampling and Analysis Plan (EA 2006) and other specific criteria in associated EPA methods were used. Section 2.0 of this data validation report lists the criteria reviewed based on EPA documents. Section 3.0 is the glossary of qualifiers used in validating the data, and Section 4.0 provides an assessment of data by methodology.

Table 1 identifies the field sample numbers, collection dates, analyses performed, and quality control (QC) samples associated with this sample delivery group (SDG). The results of these analyses are discussed in Section 4.0, Data Assessment.

TABLE 1
SAMPLE CROSS-REFERENCE TABLE
SAMPLE DELIVERY GROUP ASA0086

Field Sample ID	Lab Sample ID	Matrix	Date Collected	Analyses Performed
NEMW32C	ASA0086-01	Water	13 Jan 2009	VOC 8260B
OCPT5	ASA0086-02	Water	13 Jan 2009	VOC 8260B
TRIP BLANK	ASA0086-03	Water	13 Jan 2009	VOC 8260B
Note: VOC: volatile organic compounds				

2.0 DATA VALIDATION REQUIREMENTS

The items listed below were evaluated for the validation review.

- Chain-of-custody/sample receipt
- Holding times
- Instrument performance
- Initial and continuing calibrations
- Blanks
- Surrogate recovery
- Spikes and laboratory duplicates
- Field QC samples
- Internal standards
- Compound quantitation and reporting limits
- Overall data assessment and data qualification.

3.0 GLOSSARY OF DATA QUALIFIERS

The following definitions provide a brief explanation for data qualifiers used during the data review process. The definitions are consistent with "National Functional Guidelines for Organic Data Review" (EPA 2008).

- No Qualifier Indicates that the data are acceptable both qualitatively and quantitatively.
- U The analyte was analyzed for, but was not detected at a level greater than or equal to the level of the adjusted Contract Required Quantitation Limit (CRQL) for sample and method.
- J The analyte was positively identified and the associated numerical value is the approximate concentration of the analyte in the sample (due either to the quality of the data generated because certain quality control criteria were not met, or the concentration of the analyte was below the CRQL).
- UJ The analyte was not detected at a level greater than or equal to the adjusted CRQL. However, the reported adjusted CRQL is approximate and may be inaccurate or imprecise.
- R The sample results are unusable due to the quality of the data generated because certain criteria were not met. The analyte may or may not be present in the sample.

4.0 DATA ASSESSMENT

Analytical results were reviewed for the criteria listed in Section 2.0. A discussion of the data (by method) is presented below.

VOC 8260B

All water samples were prepared and analyzed according to the procedures set forth and specified in EPA Method 8260B for volatile organic compounds.

I. SAMPLE CONDITION/HOLDING TIMES

The sample containers were received intact at the laboratory under chain-of-custody documentation. No qualification of sample data is necessary on the basis of sample receipt or chain-of-custody.

The samples were analyzed within the 14-day holding time specified by the method.

II. GAS CHROMATOGRAPH/MASS SPECTROMETER INSTRUMENT PERFORMANCE CHECK

The analysis of the instrument performance check solution was performed at the beginning of each 12-hour period during which samples and standards were analyzed. The instrument performance check, bromofluorobenzene (BFB), met the ion abundance criteria for this SDG.

III. CALIBRATIONS

The average relative response factors met the method criteria for the system performance check compounds during the initial and continuing calibrations.

The percent relative standard deviation for the initial calibration was within the control limit of less than 15 percent for the target compounds except for iodomethane, n-butanol, and 1,2-dibromo-3-chloropropane. These compounds were not detected in the project samples, and therefore no data were qualified.

The continuing calibrations were analyzed at the proper frequency. The percent difference for the target compounds was less than the QC limit of 25 percent except for n-butanol, 1,2-dibromo-3-chloropropane, and acrolein. The following data were qualified:

- n-Butanol was qualified (UJ) in samples NEMW32C and OCPT5.
- 1,2-Dibromo-3-chloropropane was qualified (UJ) in samples NEMW32C and OCPT5.
- Acrolein was qualified (UJ) in samples NEMW32C and OCPT5.

V. BLANKS

No target compounds were detected in the method blanks. Method blanks were analyzed at the required frequency of every 12 hours, beginning with the BFB injection for each batch analyzed.

Acetone was detected in the trip blank at a concentration of 1.05 µg/L. Acetone was also detected in the project samples at a similar concentration. The following data were qualified:

- Acetone was qualified (UJ) in samples NEMW32C and OCPT5.

VI. SYSTEM MONITORING COMPOUNDS (SURROGATE RECOVERY)

The surrogates 1,2-dichloroethane-d4, toluene-d8, 4-bromofluorobenzene, and dibromofluoromthane were used as system monitoring compounds in the surrogate recovery analysis. The surrogate recoveries were within QC limits in the project samples, and no qualification was required.

VII. MATRIX SPIKE/MATRIX SPIKE DUPLICATE

The parent sample for the matrix spike/matrix spike duplicate (MS/MSD) analysis was not specific to this project. Therefore no data were qualified as a result of the MS/MSD recoveries.

VIII. LABORATORY CONTROL SAMPLE

The percent recoveries for laboratory control samples were within laboratory established control limits in this SDG. The relative percent difference for laboratory duplicate and original sample results were within laboratory-established control limits.

IX. FIELD DUPLICATE

No field duplicates were included with this SDG.

X. INTERNAL STANDARD PERFORMANCE

The internal standard areas and retention times for fluorobenzene, chlorobenzene-d5, and 1,4-dichlorobenzene-d4 were within limits for the project samples in this SDG.

XI. QUANTITATION AND REPORTED DETECTION LIMITS

The cis-1,2-dichloroethene concentration in sample NEMW32C exceeded the instrument calibration range in the initial analysis. The sample was re-analyzed for cis-1,2-dichloroethene at a dilution factor of 2. The diluted result was reported by the laboratory.

The laboratory method detection limits for 1,2-dibromo-3-chloropropane and hexachlorobutadiene were greater than the target method detection limits established for the project. However, these compounds are not identified as primary contaminants of concern. Therefore, the data in this SDG are considered useable for comparison to the potentially responsible party sample results.

XII. OVERALL ASSESSMENT OF DATA

Target compounds were qualified (UJ) by the data reviewer due to elevated percent differences in the continuing calibration as listed in Section III of this report. Acetone results were qualified (UJ) by the data reviewer due to detected acetone in the associated trip blank. Qualified data are presented in Table 2. None of the results were rejected. The data are acceptable with the qualifications noted and appended to the data by the reviewer and/or the laboratory. These qualifiers modify the usefulness of the individual values to which they are assigned.

**TABLE 2
QUALIFIED TARGET ANALYTE SUMMARY
VOLATILE ORGANIC COMPOUNDS**

Project: **Gulco Marine Maintenance Site** Matrix: **Ground water**
 SDG No.: **ASA0086** Units: **µg/L (micrograms per liter)**

Field ID	Lab ID	Analyte	Lab Reported Concentration		QA Reported Concentration		Quality Assurance Decision	Footnote
NEMW32C	ASA0086-001	n-Butanol	<13.0	ND	<13.0	UJ	Qualify	1
NEMW32C	ASA0086-001	1,2-Dibromo-3-chloropropane	<0.342	ND	<0.342	UJ	Qualify	1
NEMW32C	ASA0086-001	Acrolein	<1.29	ND	<1.29	UJ	Qualify	1
NEMW32C	ASA0086-001	Acetone	0.978	J	0.978	UJ	Qualify	2
OCPT5	ASA0086-002	n-Butanol	<13.0	ND	<13.0	UJ	Qualify	1
OCPT5	ASA0086-002	1,2-Dibromo-3-chloropropane	<0.342	ND	<0.342	UJ	Qualify	1
OCPT5	ASA0086-002	Acrolein	<1.29	ND	<1.29	UJ	Qualify	1
OCPT5	ASA0086-002	Acetone	2.31	J	2.31	UJ	Qualify	2

Notes:
 1 - The reported value has been flagged due to elevated percent difference in the continuing calibration.
 2 - Acetone was detected in the associated trip blank.
 ND - not detected
 J - concentrated value
 UJ - elevated percent difference in the continuing calibration
 QA - quality assurance
 µg/L - micrograms per liter

REFERENCES

EA Engineering, Science, and Technology, Inc. (EA). 2006. "Sampling and Analysis Plan for Remedial Investigation/Feasibility Study Oversight, Gulfco Marine Maintenance Site Freeport, Brazoria County, Texas." September.

U.S. Environmental Protection Agency (EPA). 2008. "National Functional Guidelines for Organic Data Review." June.

Enclosure 3

Analytical Data Package

RECEIVED
FEB 06 2009
EA ENG. DALLAS

Analytical Report

Work Order: ASA0086


SDG Number:

Work Order Description: Gulfco Marine EP-W-06-004

For:

Luis Vega

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067



Neal Salcher

Project Manager

Neal.Salcher@testamericainc.com

Tuesday, February 3, 2009

The test results in this report meet all NELAP requirements for analytes for which accreditation is required or available. Any exception to NELAP requirements are noted in this report. Pursuant to NELAP, this report may not be reproduced, except in full, without the written approval of the laboratory. All questions regarding this test report should be directed to the TestAmerica Project manager who has signed this report.

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfco Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

Case Narrative

Gulfco Marine

This report contains results for the received under chain-of-custody by TestAmerica Laboratories, Inc. 1/14/2009 8:30:00 AM.

These samples are associated with your T/O 0006-RSBD-06JZ project.

All samples were received in good condition and within temperature requirements.

All applicable quality control procedures met method specified acceptance criteria except where flagged on the result pages or noted in the case narrative.

Note that if this report contains tests performed for the following methods, the associated method deviations are applicable.

EPA 410.4, COD: Laboratory uses different analytical wavelength as specified by instrument manufacturer.

EPA 340.2, Fluoride: Preliminary Bellack distillation not performed.

EPA 624: The laboratory uses a different desorb time and purge volume than stated in the method.

Iowa OA 1: Benzene, toluene, ethylbenzene and xylenes (BTEX) are not analyzed along with the Gasoline Range Organics if client does not require BTEX.

EPA TO-12: Samples not analyzed in duplicate.

EPA TO-14A and TO-15: Zero humidified nitrogen is used in place of air for method blanks.

If you should have any questions, please feel free to contact me at neal.salcher@testamericainc.com or (512) 310-5215.

There are pertinent documents appended to this report, 3 pages, are included and are an integral part of this report.

Reproduction of this analytical report is permitted only in its entirety. This report shall not be reproduced except in full without the written approval of the laboratory.

TestAmerica Laboratories, Inc. certifies that the analytical results contained herein apply only to the samples tested as received by our Laboratory.

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfo Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

DATA QUALIFIERS AND DEFINITIONS

- J** Estimated value. Analyte detected at a level less than the Reporting Limit (RL) and greater than or equal to the Method Detection Limit (MDL). The user of this data should be aware that this data is of limited reliability.
- M13** The sample spiked had a pH of less than 2. 2-Chloroethylvinylether degrades under acidic conditions.
- M7** The MS and/or MSD were above the acceptance limits. See Blank Spike (LCS).
- R** The RPD exceeded the method control limit due to sample matrix effects. The individual analyte QA/QC recoveries, however, were within acceptance limits.

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfco Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

Executive Summary - Detections

Analyte	Sample Result	Data Qualifiers	Rpt Limit	MDL	Units	Dilution Factor	Date Analyzed	Analyst	Seq/ Batch	Method
Sample ID: ASA0086-01 (NEMW32C - Water)						Sampled: 01/13/09 09:15		Recvd: 01/14/09 08:30		
<u>Volatile Organic Compounds by SW846 8260B</u>										
1,1,1-Trichloroethane	0.761	J	1.00	0.360	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,1-Dichloroethane	22.7		1.00	0.374	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,1-Dichloroethene	1.46		1.00	0.427	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,2,3-Trichloropropane	5.35		1.00	0.304	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,2-Dichloroethane	0.581	J	1.00	0.392	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,2-Dichloroethene, Total	114		4.00	1.46	ug/L	2.00	01/26/09 20:17	DY	9A27008	SW846 8260B
Acetone	0.978	J	5.00	0.819	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Benzene	1.53		1.00	0.392	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Carbon disulfide	1.14		1.00	0.383	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
cis-1,2-Dichloroethene	114		2.00	0.735	ug/L	2.00	01/26/09 20:17	DY	9A27008	SW846 8260B
Tetrachloroethene	0.519	J	1.00	0.398	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Toluene	0.771	J	1.00	0.391	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
trans-1,2-Dichloroethene	0.531	J	1.00	0.372	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Trichloroethene	36.0		1.00	0.449	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Sample ID: ASA0086-02 (OCPT5 - Water)						Sampled: 01/13/09 10:00		Recvd: 01/14/09 08:30		
<u>Volatile Organic Compounds by SW846 8260B</u>										
Acetone	2.31	J	5.00	0.819	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Carbon disulfide	0.614	J	1.00	0.383	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Sample ID: ASA0086-03 (TRIP BLANK - Water)						Sampled: 01/13/09 00:01		Recvd: 01/14/09 08:30		
<u>Volatile Organic Compounds by SW846 8260B</u>										
Acetone	1.05	J	5.00	0.819	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulco Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

Sample Summary

SAMPLE IDENTIFICATION	LAB NUMBER	Client Matrix	Date/Time Sampled	Date/Time Received
NEMW32C	ASA0086-01	Water	01/13/09 09:15	01/14/09 08:30
OCPT5	ASA0086-02	Water	01/13/09 10:00	01/14/09 08:30
TRIP BLANK	ASA0086-03	Water	01/13/09 00:01	01/14/09 08:30

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfco Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

Analytical Report

Analyte	Sample Result	Data Qualifiers	Rpt Limit	MDL	Units	Dilution Factor	Date Analyzed	Analyst	Seq/ Batch	Method
Sample ID: ASA0086-01 (NEMW32C - Water)										
Volatile Organic Compounds by SW846 8260B										
						Sampled: 01/13/09 09:15		Recvd: 01/14/09 08:30		
1,1,1,2-Tetrachloroethane	ND		1.00	0.332	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,1,1-Trichloroethane	0.761	J	1.00	0.360	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,1,2,2-Tetrachloroethane	ND		1.00	0.310	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,1,2-Trichloroethane	ND		1.00	0.352	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,1,2-Trichlorotrifluoroethane	ND		1.00	0.382	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,1-Dichloroethane	22.7		1.00	0.374	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,1-Dichloroethene	1.46		1.00	0.427	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,1-Dichloropropene	ND		1.00	0.348	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,2,3-Trichloropropane	5.35		1.00	0.304	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,2,4-Trichlorobenzene	ND		1.00	0.484	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,2,4-Trimethylbenzene	ND		1.00	0.598	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,2-Dibromo-3-chloropropane	ND		5.00	0.342	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,2-Dibromoethane (EDB)	ND		1.00	0.298	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,2-Dichlorobenzene	ND		1.00	0.434	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,2-Dichloroethane	0.581	J	1.00	0.392	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,2-Dichloroethene, Total	114		4.00	1.46	ug/L	2.00	01/26/09 20:17	DY	9A27008	SW846 8260B
1,2-Dichloropropane	ND		1.00	0.373	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,3,5-Trimethylbenzene	ND		1.00	0.488	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,3-Dichlorobenzene	ND		1.00	0.386	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,3-Dichloropropane	ND		1.00	0.292	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
1,4-Dichlorobenzene	ND		1.00	0.376	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
2,2-Dichloropropane	ND		1.00	0.390	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
2-Butanone (MEK)	ND		5.00	0.841	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
2-Chloroethyl vinyl ether	ND		5.00	0.623	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
2-Chlorotoluene	ND		1.00	0.395	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
2-Hexanone	ND		5.00	0.266	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
4-Chlorotoluene	ND		1.00	0.344	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
4-Isopropyltoluene	ND		1.00	0.633	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
4-Methyl-2-pentanone (MIBK)	ND		5.00	0.416	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Acetone	0.978	J	5.00	0.819	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Acrolein	ND		10.0	1.29	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Acrylonitrile	ND		10.0	1.49	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Benzene	1.53		1.00	0.392	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Bromobenzene	ND		1.00	0.394	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Bromodichloromethane	ND		1.00	0.369	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Bromoform	ND		2.00	0.269	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Bromomethane	ND		2.00	0.723	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Carbon disulfide	1.14		1.00	0.383	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Carbon tetrachloride	ND		1.00	0.407	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Chlorobenzene	ND		1.00	0.333	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Chlorodibromomethane	ND		1.00	0.278	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Chloroethane	ND		2.00	0.449	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Chloroform	ND		1.00	0.349	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Chloromethane	ND		2.00	0.482	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
cis-1,2-Dichloroethene	114		2.00	0.735	ug/L	2.00	01/26/09 20:17	DY	9A27008	SW846 8260B
cis-1,3-Dichloropropene	ND		1.00	0.307	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Dibromomethane	ND		1.00	0.407	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Dichlorodifluoromethane	ND		2.00	0.518	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Ethylbenzene	ND		1.00	0.416	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Hexachlorobutadiene	ND		1.00	0.567	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Iodomethane	ND		1.00	0.590	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B

TestAmerica Austin

14050 Summit Drive, Suite A100 Austin, TX 78728 tel 512-244-0855 fax 512-244-0160

www.testamericainc.com

Page 6 of 17

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfo Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

Analytical Report

Analyte	Sample Result	Data Qualifiers	Rpt Limit	MDL	Units	Dilution Factor	Date Analyzed	Analyst	Seq/ Batch	Method
Sample ID: ASA0086-01 (NEMW32C - Water) - cont.						Sampled: 01/13/09 09:15		Recvd: 01/14/09 08:30		
<u>Volatile Organic Compounds by SW846 8260B - cont.</u>										
Isopropylbenzene	ND		1.00	0.418	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Methyl Acetate	ND		5.00	0.962	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Methyl tert-Butyl Ether	ND		1.00	0.336	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Methylcyclohexane	ND		5.00	0.723	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Methylene chloride	ND		1.00	0.422	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
n-Butanol	ND		250	13.0	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
n-Butylbenzene	ND		1.00	0.878	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
n-Propylbenzene	ND		1.00	0.441	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
sec-Butylbenzene	ND		1.00	0.609	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Styrene	ND		1.00	0.310	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
tert-Butylbenzene	ND		1.00	0.450	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Tetrachloroethene	0.519	J	1.00	0.398	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Toluene	0.771	J	1.00	0.391	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
trans-1,2-Dichloroethene	0.531	J	1.00	0.372	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
trans-1,3-Dichloropropene	ND		1.00	0.209	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
trans-1,4-Dichloro-2-butene	ND		5.00	0.357	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Trichloroethene	36.0		1.00	0.449	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Trichlorofluoromethane	ND		2.00	0.474	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Vinyl acetate	ND		2.00	0.293	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Vinyl chloride	ND		2.00	0.402	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Xylenes, total	ND		3.00	1.20	ug/L	1.00	01/26/09 11:32	DY	9A27008	SW846 8260B
Surr: 1,2-Dichloroethane-d4 (69-133%)	101 %						01/26/09 11:32	DY	9A27008	SW846 8260B
Surr: 1,2-Dichloroethane-d4 (69-133%)	106 %						01/26/09 20:17	DY	9A27008	SW846 8260B
Surr: 4-Bromofluorobenzene (66-124%)	109 %						01/26/09 11:32	DY	9A27008	SW846 8260B
Surr: 4-Bromofluorobenzene (66-124%)	108 %						01/26/09 20:17	DY	9A27008	SW846 8260B
Surr: Dibromofluoromethane (81-127%)	100 %						01/26/09 11:32	DY	9A27008	SW846 8260B
Surr: Dibromofluoromethane (81-127%)	101 %						01/26/09 20:17	DY	9A27008	SW846 8260B
Surr: Toluene-d8 (87-121%)	109 %						01/26/09 11:32	DY	9A27008	SW846 8260B
Surr: Toluene-d8 (87-121%)	111 %						01/26/09 20:17	DY	9A27008	SW846 8260B

TestAmerica Austin

14050 Summit Drive, Suite A100 Austin, TX 78728 tel 512-244-0855 fax 512-244-0160

www.testamericainc.com

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfco Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

Analytical Report

Analyte	Sample Result	Data Qualifiers	Rpt Limit	MDL	Units	Dilution Factor	Date Analyzed	Analyst	Seq/ Batch	Method
Sample ID: ASA0086-02 (OCPT5 - Water)						Sampled: 01/13/09 10:00		Recvd: 01/14/09 08:30		
Volatile Organic Compounds by SW846 8260B										
1,1,1,2-Tetrachloroethane	ND		1.00	0.332	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,1,1-Trichloroethane	ND		1.00	0.360	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,1,2,2-Tetrachloroethane	ND		1.00	0.310	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,1,2-Trichloroethane	ND		1.00	0.352	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,1,2-Trichlorotrifluoroethane	ND		1.00	0.382	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,1-Dichloroethane	ND		1.00	0.374	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,1-Dichloroethene	ND		1.00	0.427	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,1-Dichloropropene	ND		1.00	0.348	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,2,3-Trichloropropane	ND		1.00	0.304	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,2,4-Trichlorobenzene	ND		1.00	0.484	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,2,4-Trimethylbenzene	ND		1.00	0.598	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,2-Dibromo-3-chloropropane	ND		5.00	0.342	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,2-Dibromoethane (EDB)	ND		1.00	0.298	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,2-Dichlorobenzene	ND		1.00	0.434	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,2-Dichloroethane	ND		1.00	0.392	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,2-Dichloroethene, Total	ND		2.00	0.730	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,2-Dichloropropane	ND		1.00	0.373	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,3,5-Trimethylbenzene	ND		1.00	0.488	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,3-Dichlorobenzene	ND		1.00	0.386	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,3-Dichloropropane	ND		1.00	0.292	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
1,4-Dichlorobenzene	ND		1.00	0.376	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
2,2-Dichloropropane	ND		1.00	0.390	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
2-Butanone (MEK)	ND		5.00	0.841	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
2-Chloroethyl vinyl ether	ND		5.00	0.623	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
2-Chlorotoluene	ND		1.00	0.395	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
2-Hexanone	ND		5.00	0.266	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
4-Chlorotoluene	ND		1.00	0.344	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
4-Isopropyltoluene	ND		1.00	0.633	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
4-Methyl-2-pentanone (MIBK)	ND		5.00	0.416	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Acetone	2.31	J	5.00	0.819	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Acrolein	ND		10.0	1.29	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Acrylonitrile	ND		10.0	1.49	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Benzene	ND		1.00	0.392	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Bromobenzene	ND		1.00	0.394	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Bromodichloromethane	ND		1.00	0.369	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Bromoform	ND		2.00	0.269	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Bromomethane	ND		2.00	0.723	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Carbon disulfide	0.614	J	1.00	0.383	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Carbon tetrachloride	ND		1.00	0.407	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Chlorobenzene	ND		1.00	0.333	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Chlorodibromomethane	ND		1.00	0.278	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Chloroethane	ND		2.00	0.449	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Chloroform	ND		1.00	0.349	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Chloromethane	ND		2.00	0.482	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
cis-1,2-Dichloroethene	ND		1.00	0.367	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
cis-1,3-Dichloropropene	ND		1.00	0.307	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Dibromomethane	ND		1.00	0.407	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Dichlorodifluoromethane	ND		2.00	0.518	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Ethylbenzene	ND		1.00	0.416	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Hexachlorobutadiene	ND		1.00	0.567	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Iodomethane	ND		1.00	0.590	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B

TestAmerica Austin

14050 Summit Drive, Suite A100 Austin, TX 78728 tel 512-244-0855 fax 512-244-0160

www.testamericainc.com

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfco Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

Analytical Report

Analyte	Sample Result	Data Qualifiers	Rpt Limit	MDL	Units	Dilution Factor	Date Analyzed	Analyst	Seq/ Batch	Method
Sample ID: ASA0086-02 (OCPT5 - Water) - cont.						Sampled: 01/13/09 10:00		Recvd: 01/14/09 08:30		
<u>Volatile Organic Compounds by SW846 8260B - cont.</u>										
Isopropylbenzene	ND		1.00	0.418	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Methyl Acetate	ND		5.00	0.962	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Methyl tert-Butyl Ether	ND		1.00	0.336	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Methylcyclohexane	ND		5.00	0.723	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Methylene chloride	ND		1.00	0.422	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
n-Butanol	ND		250	13.0	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
n-Butylbenzene	ND		1.00	0.878	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
n-Propylbenzene	ND		1.00	0.441	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
sec-Butylbenzene	ND		1.00	0.609	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Styrene	ND		1.00	0.310	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
tert-Butylbenzene	ND		1.00	0.450	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Tetrachloroethene	ND		1.00	0.398	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Toluene	ND		1.00	0.391	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
trans-1,2-Dichloroethene	ND		1.00	0.372	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
trans-1,3-Dichloropropene	ND		1.00	0.209	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
trans-1,4-Dichloro-2-butene	ND		5.00	0.357	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Trichloroethene	ND		1.00	0.449	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Trichlorofluoromethane	ND		2.00	0.474	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Vinyl acetate	ND		2.00	0.293	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Vinyl chloride	ND		2.00	0.402	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Xylenes, total	ND		3.00	1.20	ug/L	1.00	01/26/09 11:59	DY	9A27008	SW846 8260B
Surr: 1,2-Dichloroethane-d4 (69-133%)	103 %						01/26/09 11:59	DY	9A27008	SW846 8260B
Surr: 4-Bromofluorobenzene (66-124%)	107 %						01/26/09 11:59	DY	9A27008	SW846 8260B
Surr: Dibromofluoromethane (81-127%)	101 %						01/26/09 11:59	DY	9A27008	SW846 8260B
Surr: Toluene-d8 (87-121%)	110 %						01/26/09 11:59	DY	9A27008	SW846 8260B
Sample ID: ASA0086-03 (TRIP BLANK - Water)						Sampled: 01/13/09 00:01		Recvd: 01/14/09 08:30		
<u>Volatile Organic Compounds by SW846 8260B</u>										
1,1,1,2-Tetrachloroethane	ND		1.00	0.332	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,1,1-Trichloroethane	ND		1.00	0.360	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,1,2,2-Tetrachloroethane	ND		1.00	0.310	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,1,2-Trichloroethane	ND		1.00	0.352	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,1,2-Trichlorotrifluoroethane	ND		1.00	0.382	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,1-Dichloroethane	ND		1.00	0.374	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,1-Dichloroethene	ND		1.00	0.427	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,1-Dichloropropene	ND		1.00	0.348	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,2,3-Trichloropropane	ND		1.00	0.304	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,2,4-Trichlorobenzene	ND		1.00	0.484	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,2,4-Trimethylbenzene	ND		1.00	0.598	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,2-Dibromo-3-chloropropane	ND		5.00	0.342	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,2-Dibromoethane (EDB)	ND		1.00	0.298	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,2-Dichlorobenzene	ND		1.00	0.434	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,2-Dichloroethane	ND		1.00	0.392	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,2-Dichloroethene, Total	ND		2.00	0.730	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,2-Dichloropropane	ND		1.00	0.373	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,3,5-Trimethylbenzene	ND		1.00	0.488	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,3-Dichlorobenzene	ND		1.00	0.386	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,3-Dichloropropane	ND		1.00	0.292	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
1,4-Dichlorobenzene	ND		1.00	0.376	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
2,2-Dichloropropane	ND		1.00	0.390	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
2-Butanone (MEK)	ND		5.00	0.841	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B

TestAmerica Austin

14050 Summit Drive, Suite A100 Austin, TX 78728 tel 512-244-0855 fax 512-244-0160

www.testamericainc.com

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfco Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

Analytical Report

Analyte	Sample Result	Data Qualifiers	Rpt Limit	MDL	Units	Dilution Factor	Date Analyzed	Analyst	Seq/ Batch	Method
Sample ID: ASA0086-03 (TRIP BLANK - Water) - cont.						Sampled: 01/13/09 00:01		Recvd: 01/14/09 08:30		
<u>Volatile Organic Compounds by SW846 8260B - cont.</u>										
2-Chloroethyl vinyl ether	ND		5.00	0.623	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
2-Chlorotoluene	ND		1.00	0.395	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
2-Hexanone	ND		5.00	0.266	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
4-Chlorotoluene	ND		1.00	0.344	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
4-Isopropyltoluene	ND		1.00	0.633	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
4-Methyl-2-pentanone (MIBK)	ND		5.00	0.416	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Acetone	1.05	J	5.00	0.819	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Acrolein	ND		10.0	1.29	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Acrylonitrile	ND		10.0	1.49	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Benzene	ND		1.00	0.392	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Bromobenzene	ND		1.00	0.394	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Bromodichloromethane	ND		1.00	0.369	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Bromofom	ND		2.00	0.269	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Bromomethane	ND		2.00	0.723	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Carbon disulfide	ND		1.00	0.383	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Carbon tetrachloride	ND		1.00	0.407	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Chlorobenzene	ND		1.00	0.333	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Chlorodibromomethane	ND		1.00	0.278	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Chloroethane	ND		2.00	0.449	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Chloroform	ND		1.00	0.349	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Chloromethane	ND		2.00	0.482	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
cis-1,2-Dichloroethene	ND		1.00	0.367	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
cis-1,3-Dichloropropene	ND		1.00	0.307	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Dibromomethane	ND		1.00	0.407	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Dichlorodifluoromethane	ND		2.00	0.518	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Ethylbenzene	ND		1.00	0.416	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Hexachlorobutadiene	ND		1.00	0.567	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Iodomethane	ND		1.00	0.590	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Isopropylbenzene	ND		1.00	0.418	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Methyl Acetate	ND		5.00	0.962	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Methyl tert-Butyl Ether	ND		1.00	0.336	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Methylcyclohexane	ND		5.00	0.723	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Methylene chloride	ND		1.00	0.422	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
n-Butanol	ND		250	13.0	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
n-Butylbenzene	ND		1.00	0.878	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
n-Propylbenzene	ND		1.00	0.441	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
sec-Butylbenzene	ND		1.00	0.609	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Styrene	ND		1.00	0.310	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
tert-Butylbenzene	ND		1.00	0.450	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Tetrachloroethene	ND		1.00	0.398	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Toluene	ND		1.00	0.391	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
trans-1,2-Dichloroethene	ND		1.00	0.372	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
trans-1,3-Dichloropropene	ND		1.00	0.209	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
trans-1,4-Dichloro-2-butene	ND		5.00	0.357	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Trichloroethene	ND		1.00	0.449	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Trichlorofluoromethane	ND		2.00	0.474	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Vinyl acetate	ND		2.00	0.293	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Vinyl chloride	ND		2.00	0.402	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Xylenes, total	ND		3.00	1.20	ug/L	1.00	01/26/09 12:26	DY	9A27008	SW846 8260B
Surr: 1,2-Dichloroethane-d4 (69-133%)	98 %						01/26/09 12:26	DY	9A27008	SW846 8260B
Surr: 4-Bromofluorobenzene (66-124%)	105 %						01/26/09 12:26	DY	9A27008	SW846 8260B

TestAmerica Austin

14050 Summit Drive, Suite A100 Austin, TX 78728 tel 512-244-0855 fax 512-244-0160

www.testamericainc.com

EA Engineering Science & Technology
 405 South Highway 121, Building C, Suite 100
 Lewisville, TX 75067

Work Order: ASA0086
 Project: Gulfco Marine
 Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
 Reported: 02/03/09 11:27

Analytical Report

Analyte	Sample Result	Data Qualifiers	Rpt Limit	MDL	Units	Dilution Factor	Date Analyzed	Analyst	Seq/ Batch	Method
Sample ID: ASA0086-03 (TRIP BLANK - Water) - cont.						Sampled: 01/13/09 00:01		Recvd: 01/14/09 08:30		
<u>Volatile Organic Compounds by SW846 8260B - cont.</u>										
<i>Surr: Dibromofluoromethane (81-127%)</i>	98 %						01/26/09 12:26	DY	9A27008	SW846 8260B
<i>Surr: Toluene-d8 (87-121%)</i>	108 %						01/26/09 12:26	DY	9A27008	SW846 8260B

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfco Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

LABORATORY BLANK QC DATA

Analyte	Seq/ Batch	Spike Level	MRL	MDL	Units	Result	Dup Result	% REC	Dup %REC	% REC Limits	RPD RPD	RPD Limit	Q
Volatle Organic Compounds by SW846 8260B													
1,1,1,2-Tetrachloroethane	9A27008		1.00	0.332	ug/L	ND							
1,1,1-Trichloroethane	9A27008		1.00	0.360	ug/L	ND							
1,1,2,2-Tetrachloroethane	9A27008		1.00	0.310	ug/L	ND							
1,1,2-Trichloroethane	9A27008		1.00	0.352	ug/L	ND							
1,1,2-Trichlorotrifluoroethane	9A27008		1.00	0.382	ug/L	ND							
1,1-Dichloroethane	9A27008		1.00	0.374	ug/L	ND							
1,1-Dichloroethene	9A27008		1.00	0.427	ug/L	ND							
1,1-Dichloropropene	9A27008		1.00	0.348	ug/L	ND							
1,2,3-Trichloropropane	9A27008		1.00	0.304	ug/L	ND							
1,2,4-Trichlorobenzene	9A27008		1.00	0.484	ug/L	ND							
1,2,4-Trimethylbenzene	9A27008		1.00	0.598	ug/L	ND							
1,2-Dibromo-3-chloropropane	9A27008		5.00	0.342	ug/L	ND							
1,2-Dibromoethane (EDB)	9A27008		1.00	0.298	ug/L	ND							
1,2-Dichlorobenzene	9A27008		1.00	0.434	ug/L	ND							
1,2-Dichloroethane	9A27008		1.00	0.392	ug/L	ND							
1,2-Dichloroethene, Total	9A27008		2.00	0.730	ug/L	ND							
1,2-Dichloropropane	9A27008		1.00	0.373	ug/L	ND							
1,3,5-Trimethylbenzene	9A27008		1.00	0.488	ug/L	ND							
1,3-Dichlorobenzene	9A27008		1.00	0.386	ug/L	ND							
1,3-Dichloropropane	9A27008		1.00	0.292	ug/L	ND							
1,4-Dichlorobenzene	9A27008		1.00	0.376	ug/L	ND							
2,2-Dichloropropane	9A27008		1.00	0.390	ug/L	ND							
2-Butanone (MEK)	9A27008		5.00	0.841	ug/L	ND							
2-Chloroethyl vinyl ether	9A27008		5.00	0.623	ug/L	ND							
2-Chlorotoluene	9A27008		1.00	0.395	ug/L	ND							
2-Hexanone	9A27008		5.00	0.266	ug/L	ND							
4-Chlorotoluene	9A27008		1.00	0.344	ug/L	ND							
4-Isopropyltoluene	9A27008		1.00	0.633	ug/L	ND							
4-Methyl-2-pentanone (MIBK)	9A27008		5.00	0.416	ug/L	ND							
Acetone	9A27008		5.00	0.819	ug/L	ND							
Acrolein	9A27008		10.0	1.29	ug/L	ND							
Acrylonitrile	9A27008		10.0	1.49	ug/L	ND							
Benzene	9A27008		1.00	0.392	ug/L	ND							
Bromobenzene	9A27008		1.00	0.394	ug/L	ND							
Bromodichloromethane	9A27008		1.00	0.369	ug/L	ND							
Bromoform	9A27008		2.00	0.269	ug/L	ND							
Bromomethane	9A27008		2.00	0.723	ug/L	ND							
Carbon disulfide	9A27008		1.00	0.383	ug/L	ND							
Carbon tetrachloride	9A27008		1.00	0.407	ug/L	ND							
Chlorobenzene	9A27008		1.00	0.333	ug/L	ND							
Chlorodibromomethane	9A27008		1.00	0.278	ug/L	ND							
Chloroethane	9A27008		2.00	0.449	ug/L	ND							
Chloroform	9A27008		1.00	0.349	ug/L	ND							
Chloromethane	9A27008		2.00	0.482	ug/L	ND							
cis-1,2-Dichloroethene	9A27008		1.00	0.367	ug/L	ND							

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfoo Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

LABORATORY BLANK QC DATA

Analyte	Seq/ Batch	Spike Level	MRL	MDL	Units	Result	Dup Result	% REC	Dup %REC	% REC Limits	RPD RPD	Limit	Q
Volatile Organic Compounds by SW846 8260B													
cis-1,3-Dichloropropene	9A27008		1.00	0.307	ug/L	ND							
Dibromomethane	9A27008		1.00	0.407	ug/L	ND							
Dichlorodifluoromethane	9A27008		2.00	0.518	ug/L	ND							
Ethylbenzene	9A27008		1.00	0.416	ug/L	ND							
Hexachlorobutadiene	9A27008		1.00	0.567	ug/L	ND							
Iodomethane	9A27008		1.00	0.590	ug/L	ND							
Isopropylbenzene	9A27008		1.00	0.418	ug/L	ND							
Methyl Acetate	9A27008		5.00	0.962	ug/L	ND							
Methyl tert-Butyl Ether	9A27008		1.00	0.336	ug/L	ND							
Methylcyclohexane	9A27008		5.00	0.723	ug/L	ND							
Methylene chloride	9A27008		1.00	0.422	ug/L	ND							
n-Butanol	9A27008		250	13.0	ug/L	ND							
n-Butylbenzene	9A27008		1.00	0.878	ug/L	ND							
n-Propylbenzene	9A27008		1.00	0.441	ug/L	ND							
sec-Butylbenzene	9A27008		1.00	0.609	ug/L	ND							
Styrene	9A27008		1.00	0.310	ug/L	ND							
tert-Butylbenzene	9A27008		1.00	0.450	ug/L	ND							
Tetrachloroethene	9A27008		1.00	0.398	ug/L	ND							
Toluene	9A27008		1.00	0.391	ug/L	ND							
trans-1,2-Dichloroethene	9A27008		1.00	0.372	ug/L	ND							
trans-1,3-Dichloropropene	9A27008		1.00	0.209	ug/L	ND							
trans-1,4-Dichloro-2-butene	9A27008		5.00	0.357	ug/L	ND							
Trichloroethene	9A27008		1.00	0.449	ug/L	ND							
Trichlorofluoromethane	9A27008		2.00	0.474	ug/L	ND							
Vinyl acetate	9A27008		2.00	0.293	ug/L	ND							
Vinyl chloride	9A27008		2.00	0.402	ug/L	ND							
Xylenes, total	9A27008		3.00	1.20	ug/L	ND							
Surrogate:	9A27008				ug/L			92		69-133			
1,2-Dichloroethane-d4													
Surrogate:	9A27008				ug/L			105		66-124			
4-Bromofluorobenzene													
Surrogate:	9A27008				ug/L			94		81-127			
Dibromofluoromethane													
Surrogate: Toluene-d8	9A27008				ug/L			108		87-121			

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfco Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

LCS/LCS DUPLICATE QC DATA

Analyte	Seq/ Batch	Spike Level	MRL	MDL	Units	Result	Dup Result	% REC	Dup %REC	% REC Limits	RPD RPD	RPD Limit	Q
Volatile Organic Compounds by SW846 8260B													
1,1,1,2-Tetrachloroethane	9A27008	20.00	1.00	0.332	ug/L	19.1	18.3	96	91	66-137	4	20	
1,1,1-Trichloroethane	9A27008	20.00	1.00	0.360	ug/L	21.8	20.8	109	104	69-141	5	20	
1,1,2,2-Tetrachloroethane	9A27008	20.00	1.00	0.310	ug/L	17.7	16.8	89	84	61-128	5	20	
1,1,2-Trichloroethane	9A27008	20.00	1.00	0.352	ug/L	16.6	15.9	83	79	67-142	4	20	
1,1,2-Trichlorotrifluoroethane	9A27008	20.00	1.00	0.382	ug/L	22.9	22.0	114	110	58-121	4	20	
1,1-Dichloroethane	9A27008	20.00	1.00	0.374	ug/L	22.0	20.7	110	104	65-134	6	20	
1,1-Dichloroethene	9A27008	20.00	1.00	0.427	ug/L	20.4	19.6	102	98	62-135	4	20	
1,1-Dichloropropene	9A27008	20.00	1.00	0.348	ug/L	25.5	22.5	117	112	64-132	4	20	
1,2,3-Trichloropropane	9A27008	20.00	1.00	0.304	ug/L	15.3	14.4	77	72	68-140	6	20	
1,2,4-Trichlorobenzene	9A27008	20.00	1.00	0.484	ug/L	20.5	19.9	102	99	10-141	3	20	
1,2,4-Trimethylbenzene	9A27008	20.00	1.00	0.598	ug/L	20.1	19.4	100	97	66-138	4	20	
1,2-Dibromo-3-chloropropane	9A27008	20.00	5.00	0.342	ug/L	12.5	11.9	62	59	52-109	5	20	
1,2-Dibromoethane (EDB)	9A27008	20.00	1.00	0.298	ug/L	16.8	16.2	84	81	67-141	4	20	
1,2-Dichlorobenzene	9A27008	20.00	1.00	0.434	ug/L	18.8	17.9	94	89	63-130	5	20	
1,2-Dichloroethane	9A27008	20.00	1.00	0.392	ug/L	21.5	20.4	107	102	66-137	5	20	
1,2-Dichloroethene, Total	9A27008	40.00	2.00	0.730	ug/L	40.9	39.2	102	98	64-133	4	20	
1,2-Dichloropropane	9A27008	20.00	1.00	0.373	ug/L	21.5	20.5	108	102	80-120	5	20	
1,3,5-Trimethylbenzene	9A27008	20.00	1.00	0.488	ug/L	20.2	19.4	101	97	67-140	4	20	
1,3-Dichlorobenzene	9A27008	20.00	1.00	0.386	ug/L	19.2	18.4	96	92	63-131	5	20	
1,3-Dichloropropane	9A27008	20.00	1.00	0.292	ug/L	17.5	16.8	88	84	66-136	4	20	
1,4-Dichlorobenzene	9A27008	20.00	1.00	0.376	ug/L	18.5	17.8	93	89	62-128	4	20	
2,2-Dichloropropane	9A27008	20.00	1.00	0.390	ug/L	21.3	20.2	106	101	23-176	5	20	
2-Butanone (MEK)	9A27008	20.00	5.00	0.841	ug/L	18.0	16.1	90	81	50-150	11	20	
2-Chloroethyl vinyl ether	9A27008	20.02	5.00	0.623	ug/L	18.2	17.2	91	86	10-200	6	20	
2-Chlorotoluene	9A27008	20.00	1.00	0.395	ug/L	20.0	19.6	100	98	63-147	2	20	
2-Hexanone	9A27008	20.00	5.00	0.266	ug/L	17.0	16.2	85	81	50-150	5	20	
4-Chlorotoluene	9A27008	20.00	1.00	0.344	ug/L	20.0	19.3	100	96	70-140	4	20	
4-Isopropyltoluene	9A27008	20.00	1.00	0.633	ug/L	20.5	19.8	102	99	63-131	3	20	
4-Methyl-2-pentanone (MIBK)	9A27008	20.00	5.00	0.416	ug/L	18.4	17.9	92	89	62-128	3	20	
Acetone	9A27008	20.00	5.00	0.819	ug/L	16.0	15.4	80	77	71-194	4	20	
Acrolein	9A27008	100.1	10.0	1.29	ug/L	119	116	119	116	10-200	3	20	
Acrylonitrile	9A27008	100.0	10.0	1.49	ug/L	89.1	86.4	89	86	67-138	3	20	
Benzene	9A27008	20.00	1.00	0.392	ug/L	21.7	20.8	108	104	64-133	4	20	
Bromobenzene	9A27008	20.00	1.00	0.394	ug/L	19.7	18.8	99	94	63-131	5	20	
Bromodichloromethane	9A27008	20.00	1.00	0.369	ug/L	20.2	19.1	101	95	65-135	6	20	
Bromoform	9A27008	20.00	2.00	0.269	ug/L	18.1	17.1	90	85	60-125	6	20	
Bromomethane	9A27008	20.00	2.00	0.723	ug/L	22.5	22.3	112	111	40-187	1	20	
Carbon disulfide	9A27008	20.00	1.00	0.383	ug/L	22.4	21.5	112	107	64-132	4	20	
Carbon tetrachloride	9A27008	20.00	1.00	0.407	ug/L	23.2	21.8	116	109	59-134	6	20	
Chlorobenzene	9A27008	20.00	1.00	0.333	ug/L	19.6	18.8	98	94	63-132	4	20	
Chlorodibromomethane	9A27008	20.00	1.00	0.278	ug/L	17.8	17.0	89	85	65-136	5	20	
Chloroethane	9A27008	20.00	2.00	0.449	ug/L	22.3	21.5	112	107	39-142	4	20	
Chloroform	9A27008	20.00	1.00	0.349	ug/L	20.0	18.9	100	95	80-120	6	20	
Chloromethane	9A27008	20.00	2.00	0.482	ug/L	21.0	21.1	105	106	64-134	1	20	
cis-1,2-Dichloroethene	9A27008	20.00	1.00	0.367	ug/L	19.6	18.9	98	94	67-133	4	20	

TestAmerica Austin

14050 Summit Drive, Suite A100 Austin, TX 78728 tel 512-244-0855 fax 512-244-0160

www.testamericainc.com

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfo Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

LCS/LCS DUPLICATE QC DATA

Analyte	Seq/ Batch	Spike Level	MRL	MDL	Units	Result	Dup Result	% REC	Dup %REC	% REC Limits	RPD	RPD Limit	Q
Volatile Organic Compounds by SW846.8260B													
cis-1,3-Dichloropropene	9A27008	20.00	1.00	0.307	ug/L	21.2	20.3	106	101	84-124	5	20	
Dibromomethane	9A27008	20.00	1.00	0.407	ug/L	18.9	17.9	94	89	65-137	5	20	
Dichlorodifluoromethane	9A27008	20.00	2.00	0.518	ug/L	20.7	19.7	103	99	16-139	5	20	
Ethylbenzene	9A27008	20.00	1.00	0.416	ug/L	20.4	19.7	102	98	77-116	4	20	
Hexachlorobutadiene	9A27008	20.00	1.00	0.567	ug/L	19.2	18.8	96	94	10-154	2	20	
Iodomethane	9A27008	20.00	1.00	0.590	ug/L	19.1	17.3	95	87	71-147	10	20	
Isopropylbenzene	9A27008	20.00	1.00	0.418	ug/L	22.6	21.7	113	109	63-130	4	20	
Methyl Acetate	9A27008	50.00	5.00	0.962	ug/L	44.3	43.5	89	87	10-150	2	20	
Methyl tert-Butyl Ether	9A27008	20.00	1.00	0.336	ug/L	17.6	17.1	88	85	55-114	3	20	
Methylcyclohexane	9A27008	50.00	5.00	0.723	ug/L	61.3	59.1	123	118	47-141	4	20	
Methylene chloride	9A27008	20.00	1.00	0.422	ug/L	18.3	17.6	91	88	67-139	4	20	
n-Butanol	9A27008	1000	250	13.0	ug/L	458	421	46	42	10-200	8	20	
n-Butylbenzene	9A27008	20.00	1.00	0.878	ug/L	20.3	19.4	102	97	43-134	4	20	
n-Propylbenzene	9A27008	20.00	1.00	0.441	ug/L	20.5	19.5	102	98	60-125	5	20	
sec-Butylbenzene	9A27008	20.00	1.00	0.609	ug/L	21.8	21.0	109	105	63-131	3	20	
Styrene	9A27008	20.00	1.00	0.310	ug/L	21.6	20.4	108	102	58-127	5	20	
tert-Butylbenzene	9A27008	20.00	1.00	0.450	ug/L	21.1	20.1	105	100	68-140	5	20	
Tetrachloroethene	9A27008	20.00	1.00	0.398	ug/L	18.2	17.6	91	88	47-146	4	20	
Toluene	9A27008	20.00	1.00	0.391	ug/L	19.9	19.0	99	95	80-123	5	20	
trans-1,2-Dichloroethene	9A27008	20.00	1.00	0.372	ug/L	21.2	20.3	106	102	63-132	4	20	
trans-1,3-Dichloropropene	9A27008	20.00	1.00	0.209	ug/L	18.8	17.7	94	89	70-145	6	20	
trans-1,4-Dichloro-2-butene	9A27008	20.00	5.00	0.357	ug/L	20.9	19.7	105	98	43-130	6	20	
Trichloroethene	9A27008	20.00	1.00	0.449	ug/L	20.5	19.8	103	99	65-134	4	20	
Trichlorofluoromethane	9A27008	20.00	2.00	0.474	ug/L	23.2	22.2	116	111	44-132	5	20	
Vinyl acetate	9A27008	19.99	2.00	0.293	ug/L	22.4	21.4	112	107	73-150	4	20	
Vinyl chloride	9A27008	20.00	2.00	0.402	ug/L	23.2	22.0	116	110	53-139	5	20	
Xylenes, total	9A27008	60.00	3.00	1.20	ug/L	62.4	59.6	104	99	64-132	5	20	
Surrogate:	9A27008				ug/L			99	94	69-133			
1,2-Dichloroethane-d4													
Surrogate:	9A27008				ug/L			103	101	66-124			
4-Bromofluorobenzene													
Surrogate:	9A27008				ug/L			101	98	81-127			
Dibromofluoromethane													
Surrogate: Toluene-d8	9A27008				ug/L			112	109	87-121			

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfco Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

MATRIX SPIKE/MATRIX SPIKE DUPLICATE QC DATA

Analyte	Seq/ Batch	Source Result	Spike Level	MRL	MDL	Units	Result	Dup Result	% REC	Dup %REC	% REC Limits	RPD	RPD Limit	Q
Volatile Organic Compounds by SW846 8260B														
QC Source Sample: ASA0148-01														
1,1,1,2-Tetrachloroethane	9A27008	ND	20.00	1.00	0.332	ug/L	18.4	19.2	92	96	66-137	4	20	
1,1,1-Trichloroethane	9A27008	ND	20.00	1.00	0.360	ug/L	22.3	22.6	111	113	69-141	2	20	
1,1,2,2-Tetrachloroethane	9A27008	ND	20.00	1.00	0.310	ug/L	16.0	17.4	80	87	61-128	9	20	
1,1,2-Trichloroethane	9A27008	ND	20.00	1.00	0.352	ug/L	15.4	16.5	77	83	67-142	7	20	
1,1,2-Trichlorotrifluoroethane	9A27008	ND	20.00	1.00	0.382	ug/L	24.3	24.5	122	123	58-121	1	20	M7
1,1-Dichloroethane	9A27008	ND	20.00	1.00	0.374	ug/L	21.9	22.2	109	111	65-134	2	20	
1,1-Dichloroethene	9A27008	ND	20.00	1.00	0.427	ug/L	21.6	22.2	108	111	62-135	3	20	
1,1-Dichloropropene	9A27008	ND	20.00	1.00	0.348	ug/L	24.4	24.5	122	123	64-132	1	20	
1,2,3-Trichloropropane	9A27008	ND	20.00	1.00	0.304	ug/L	13.8	14.7	69	73	68-140	6	20	
1,2,4-Trichlorobenzene	9A27008	ND	20.00	1.00	0.484	ug/L	20.3	21.1	101	106	10-141	4	20	
1,2,4-Trimethylbenzene	9A27008	ND	20.00	1.00	0.598	ug/L	20.2	20.0	101	100	66-138	1	20	
1,2-Dibromo-3-chloropropane	9A27008	ND	20.00	5.00	0.342	ug/L	11.5	13.2	58	66	52-109	13	20	
1,2-Dibromoethane (EDB)	9A27008	ND	20.00	1.00	0.298	ug/L	15.8	16.9	79	85	67-141	7	20	
1,2-Dichlorobenzene	9A27008	ND	20.00	1.00	0.434	ug/L	18.1	18.7	90	94	63-130	4	20	
1,2-Dichloroethane	9A27008	ND	20.00	1.00	0.392	ug/L	19.9	21.2	100	106	66-137	6	20	
1,2-Dichloroethene, Total	9A27008	ND	40.00	2.00	0.730	ug/L	41.9	42.7	105	107	64-133	2	20	
1,2-Dichloropropane	9A27008	ND	20.00	1.00	0.373	ug/L	20.8	21.7	104	108	80-120	4	20	
1,3,5-Trimethylbenzene	9A27008	ND	20.00	1.00	0.488	ug/L	20.6	20.2	103	101	67-140	2	20	
1,3-Dichlorobenzene	9A27008	ND	20.00	1.00	0.386	ug/L	19.1	19.5	95	98	63-131	2	20	
1,3-Dichloropropane	9A27008	ND	20.00	1.00	0.292	ug/L	16.2	17.3	81	86	66-136	7	20	
1,4-Dichlorobenzene	9A27008	ND	20.00	1.00	0.376	ug/L	18.2	18.7	91	94	62-128	3	20	
2,2-Dichloropropane	9A27008	ND	20.00	1.00	0.390	ug/L	21.9	22.1	110	111	23-176	1	20	
2-Butanone (MEK)	9A27008	ND	20.00	5.00	0.841	ug/L	15.4	17.9	77	89	50-150	15	20	
2-Chloroethyl vinyl ether	9A27008	ND	20.02	5.00	0.623	ug/L	ND	<0.623			10-200		20	M13
2-Chlorotoluene	9A27008	ND	20.00	1.00	0.395	ug/L	20.5	20.4	103	102	63-147	0	20	
2-Hexanone	9A27008	ND	20.00	5.00	0.266	ug/L	15.0	17.7	75	88	50-150	16	20	
4-Chlorotoluene	9A27008	ND	20.00	1.00	0.344	ug/L	20.3	20.3	101	102	70-140	0	20	
4-Isopropyltoluene	9A27008	ND	20.00	1.00	0.633	ug/L	21.2	20.9	106	105	63-131	1	20	
4-Methyl-2-pentanone (MIBK)	9A27008	ND	20.00	5.00	0.416	ug/L	16.5	19.2	83	96	62-128	15	20	
Acetone	9A27008	0.889	20.00	5.00	0.819	ug/L	15.6	16.8	73	79	71-194	7	20	
Acrolein	9A27008	ND	100.1	10.0	1.29	ug/L	114	127	114	127	10-200	11	20	
Acrylonitrile	9A27008	ND	100.0	10.0	1.49	ug/L	83.4	94.4	83	94	67-138	12	20	
Benzene	9A27008	ND	20.00	1.00	0.392	ug/L	21.7	22.2	109	111	64-133	2	20	
Bromobenzene	9A27008	ND	20.00	1.00	0.394	ug/L	19.0	19.8	95	99	63-131	4	20	
Bromodichloromethane	9A27008	0.494	20.00	1.00	0.369	ug/L	19.9	20.8	97	102	65-135	5	20	
Bromoform	9A27008	0.584	20.00	2.00	0.269	ug/L	17.4	18.5	84	90	60-125	7	20	
Bromomethane	9A27008	ND	20.00	2.00	0.723	ug/L	24.6	26.0	123	130	40-187	6	20	
Carbon disulfide	9A27008	ND	20.00	1.00	0.383	ug/L	24.2	23.9	121	120	64-132	1	20	
Carbon tetrachloride	9A27008	ND	20.00	1.00	0.407	ug/L	23.7	23.8	119	119	59-134	1	20	
Chlorobenzene	9A27008	ND	20.00	1.00	0.333	ug/L	19.4	19.8	97	99	63-132	2	20	
Chlorodibromomethane	9A27008	0.805	20.00	1.00	0.278	ug/L	17.4	18.6	83	89	65-136	7	20	
Chloroethane	9A27008	ND	20.00	2.00	0.449	ug/L	22.9	23.5	114	118	39-142	3	20	
Chloroform	9A27008	0.469	20.00	1.00	0.349	ug/L	20.0	20.6	98	101	80-120	3	20	
Chloromethane	9A27008	ND	20.00	2.00	0.482	ug/L	24.1	24.7	120	123	64-134	2	20	
cis-1,2-Dichloroethene	9A27008	ND	20.00	1.00	0.367	ug/L	19.8	20.4	99	102	67-133	3	20	

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfco Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

MATRIX SPIKE/MATRIX SPIKE DUPLICATE QC DATA

Analyte	Seq/ Batch	Source Result	Spike Level	MRL	MDL	Units	Result	Dup Result	% REC	Dup %REC	% REC Limits	RPD	RPD Limit	Q
Volatile Organic Compounds by SW846 8260B														
QC Source Sample: ASA0148-01														
cis-1,3-Dichloropropene	9A27008	ND	20.00	1.00	0.307	ug/L	20.2	21.1	101	105	84-124	4	20	
Dibromomethane	9A27008	ND	20.00	1.00	0.407	ug/L	17.7	19.0	89	95	65-137	7	20	
Dichlorodifluoromethane	9A27008	ND	20.00	2.00	0.518	ug/L	21.8	22.3	109	112	16-139	2	20	
Ethylbenzene	9A27008	ND	20.00	1.00	0.416	ug/L	20.5	20.9	102	105	77-116	2	20	
Hexachlorobutadiene	9A27008	ND	20.00	1.00	0.567	ug/L	21.2	20.3	106	101	10-154	4	20	
Iodomethane	9A27008	ND	20.00	1.00	0.590	ug/L	18.3	17.8	91	89	71-147	2	20	
Isopropylbenzene	9A27008	ND	20.00	1.00	0.418	ug/L	22.9	23.1	115	115	63-130	1	20	
Methyl Acetate	9A27008	ND	50.00	5.00	0.962	ug/L	42.7	48.4	85	97	10-150	13	20	
Methyl tert-Butyl Ether	9A27008	ND	20.00	1.00	0.336	ug/L	16.5	18.5	83	92	55-114	11	20	
Methylcyclohexane	9A27008	ND	50.00	5.00	0.723	ug/L	64.9	65.1	130	130	47-141	0	20	
Methylene chloride	9A27008	ND	20.00	1.00	0.422	ug/L	18.0	18.7	90	93	67-139	4	20	
n-Butanol	9A27008	ND	1000	250	13.0	ug/L	375	554	37	55	10-200	39	20	R
n-Butylbenzene	9A27008	ND	20.00	1.00	0.878	ug/L	21.2	20.9	106	104	43-134	2	20	
n-Propylbenzene	9A27008	ND	20.00	1.00	0.441	ug/L	20.6	20.9	103	105	60-125	1	20	
sec-Butylbenzene	9A27008	ND	20.00	1.00	0.609	ug/L	22.7	22.2	114	111	63-131	2	20	
Styrene	9A27008	ND	20.00	1.00	0.310	ug/L	21.1	21.6	105	108	58-127	3	20	
tert-Butylbenzene	9A27008	ND	20.00	1.00	0.450	ug/L	21.2	21.3	106	106	68-140	0	20	
Tetrachloroethene	9A27008	ND	20.00	1.00	0.398	ug/L	19.3	19.3	97	96	47-146	0	20	
Toluene	9A27008	ND	20.00	1.00	0.391	ug/L	19.9	20.1	99	100	80-123	1	20	
trans-1,2-Dichloroethene	9A27008	ND	20.00	1.00	0.372	ug/L	22.1	22.3	110	112	63-132	1	20	
trans-1,3-Dichloropropene	9A27008	ND	20.00	1.00	0.209	ug/L	17.4	18.6	87	93	70-145	7	20	
trans-1,4-Dichloro-2-butene	9A27008	ND	20.00	5.00	0.357	ug/L	18.5	19.1	93	95	43-130	3	20	
Trichloroethene	9A27008	ND	20.00	1.00	0.449	ug/L	21.1	21.5	106	107	65-134	2	20	
Trichlorofluoromethane	9A27008	ND	20.00	2.00	0.474	ug/L	24.1	24.3	120	121	44-132	1	20	
Vinyl acetate	9A27008	ND	19.99	2.00	0.293	ug/L	20.7	22.6	104	113	73-150	9	20	
Vinyl chloride	9A27008	ND	20.00	2.00	0.402	ug/L	24.4	24.6	122	123	53-139	1	20	
Xylenes, total	9A27008	ND	60.00	3.00	1.20	ug/L	62.4	62.7	104	105	64-132	1	20	
Surrogate:	9A27008					ug/L			91	98	69-133			
1,2-Dichloroethane-d4						ug/L			101	102	66-124			
Surrogate:	9A27008					ug/L			97	100	81-127			
4-Bromofluorobenzene						ug/L			108	110	87-121			
Surrogate:	9A27008					ug/L								
Dibromofluoromethane						ug/L								
Surrogate: Toluene-d8	9A27008					ug/L								

CHAIN-OF-CUSTODY ADDENDUM

CHECKED/RECEIVED BY: [Signature]

Lot No: ASA0086

DATE/TIME RECEIVED: 1/24/09 08:30

COC NUMBER: _____

UNPACKED DATE/TIME: 1/24/09 09:50

QUOTE/PROFILE: _____

CLIENT/PROJECT: EA Engineering

SAMPLES LOGGED IN: _____ LOG-IN REVIEWED: _____

Number of Shipping Containers Received with Chain of Custody _____

CC JNS

VOC AIR / FILTER SAMPLES YES SEE SECTIONS 1.0, 2.0, & 6.0

1.0 CONTAINERS EXAMINED UPON RECEIPT: CC

Container Sealed: YES NO Custody Seal Signed/Dated: YES NO

Custody Seal Present: YES NO

If seal not intact list air bill number of that container(s): _____

2.0 VOC CANISTERS EXAMINED UPON RECEIPT: _____

Canister Valves Closed: YES NO Samples Received Match Chain: YES NO

Canister Valves Capped: YES NO Other Equipment Received: YES NO

Valve Cap Tightened Properly: YES NO See Additional Comments (Section 5.0 and / or 7.0) YES NO

Packing Material Used: (circle) Chain-of-Custody form properly maintained: YES NO

None / Absorbent / Paper / Bubble Wrap Can Size: 6L 15L Other _____

3.0 SAMPLE TEMPERATURE UPON RECEIPT BY: CC IR THERMOMETER #: P4 P5

Temperature of the container(s): _____

Circle selection: TB = Temp. Blank and/or SC = Sample Container CF = Correction Factor [acceptable tolerance 4°C ± 2°]

TB	SC	TB	SC	TB	SC	TB	SC	TB	SC	TB	SC	TB	SC
Initial	2.16	Initial		Initial		Initial		Initial		Initial		Initial	
CF	-0.2	CF		CF		CF		CF		CF		CF	
Final	1.42	Final		Final		Final		Final		Final		Final	

If temperature is outside acceptable tolerance, Project Manager was notified (_____ PM). Date: _____ Time: _____

Samples received do not require cooling _____ OK to analyze samples: YES NO

PRESERVATION OF SAMPLES REQUIRED: NA YES VOA Samples VERIFIED BY: [Signature]

NOTE: pH CHECK OF SAMPLES FOR 1664A ANALYSIS CHECK AT TIME OF ANALYSIS BY BENCH ANALYST
pH CHECK OF VOLATILE SAMPLES PERFORMED AFTER ANALYSIS BY THE BENCH ANALYST.

Base samples are >pH 12: YES NO Acid preserved are <pH 2: YES NO

Cyanide samples checked for sulfides: YES Sulfide samples appear to be preserved with zinc acetate: YES NO

Samples checked for chlorine per specification (N.C.) YES Free chlorine present: YES NO

If sample preservation is outside acceptable tolerance, Project Manager was notified (_____ PM)

Date: _____ Time: _____ see pH adjustment form

VOLATILE SAMPLES FILLED COMPLETELY, IF NOT, LIST ID AND HEADSPACE OF VOA'S CONTAINING BUBBLES EXCEEDING 6MM IN DIAMETER:

Sample ID	mm Headspace

Sample ID	mm Headspace

CHAIN-OF-CUSTODY ADDENDUM

Lot No: ASA 0086

4.0 CONDITION OF BOTTLES/CONTAINERS

VERIFIED BY: cc

Samples received match COC: YES NO Bottles received intact: YES NO
 See additional discrepancies/comments section: YES NO Samples received from USDA restricted area: YES NO
 Chain-of-Custody form properly maintained: YES NO VOA trip blanks included: 2 YES NO N/A

5.0 ADDITIONAL DISCREPANCIES

Appears on COC		Appears on Label		Comments
Sample ID	Date/Time	Sample ID	Date/Time	

6.0 SHIPPING DOCUMENTATION:

Air/freight bill is available and attached to COC: YES NO Air bill #: _____
 Hand-delivered Carrier: _____ Date: _____ Time: _____

7.0 OTHER COMMENTS:

CORRECTIVE ACTION:

Client's Name: _____ Informed verbally on: _____ By: _____
 Client's Name: _____ Informed verbally on: _____ By: _____
 Sample(s) processed "as is" comments: _____

Samples(s) on hold until: _____ If released, notify: _____

REVIEW:
 Project Management: *Mark [Signature]* Date: 1/16/09

SIGNED ORIGINAL MUST BE RETAINED IN THE PROJECT FILE

Supporting Documentation

Lot Number ASA 0086

(Note: A one-page "Description of Supporting Documentation" is provided at the beginning of each section.)

Check below when supporting documentation is present.

GC/MS Volatile

GC/MS Semivolatile

GC Volatile

GC Semivolatile

Metals

General Chemistry

TestAmerica

THE LEADER IN ENVIRONMENTAL TESTING

EA Engineering Science & Technology
405 South Highway 121, Building C, Suite 100
Lewisville, TX 75067

Work Order: ASA0086
Project: Gulfco Marine
Project Number: T/O 0006-RSBD-06JZ

Received: 01/14/09
Reported: 02/03/09 11:27

Sample Summary

SAMPLE IDENTIFICATION	LAB NUMBER	Client Matrix	Date/Time Sampled	Date/Time Received
NEMW32C	ASA0086-01	Water	01/13/09 09:15	01/14/09 08:30
OCPTS	ASA0086-02	Water	01/13/09 10:00	01/14/09 08:30
TRIP BLANK	ASA0086-03	Water	01/13/09 00:01	01/14/09 08:30

Metals by Method SW-846 6020 TerminologyINSTRUMENT

QC Std #1	ICV (Initial Calibration Verification)
QC Std #2	ICB (initial Calibration Blank)
QC Std #3	LLCk Std (Low-level Check Standard for TRRP only)
QC Std #4	ICSA (Interference Check Standard – Interfering Elements)
QC Std #5	ICSAB (Interference Check Standard – Analytes and Interferants)
QC Std #6	CCV (Continuing Calibration Verification)
QC Std #7	CCB (Continuing Calibration Blank)
SD5X	Serial Dilution
AS1.04X	Analytical Spike

GC/MS VOLATILES

SUPPORTING DOCUMENTATION DESCRIPTION PAGE

QC & Sample Data

Calibration Data



Method: 8240 B

Associated Samples: 1-3

Batch Number: 9A27008

BFB

Data File : C:\HPCHEM\1\DATA\I012609.B\I126903.D Vial: 3
 Acq On : 26 Jan 2009 6:26 am Operator: DY
 Sample : CCV,REG Inst : MSI
 Misc : 9010191 5uL/50mL Multiplr: 1.00
 MS Integration Params: VOA.P
 Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water

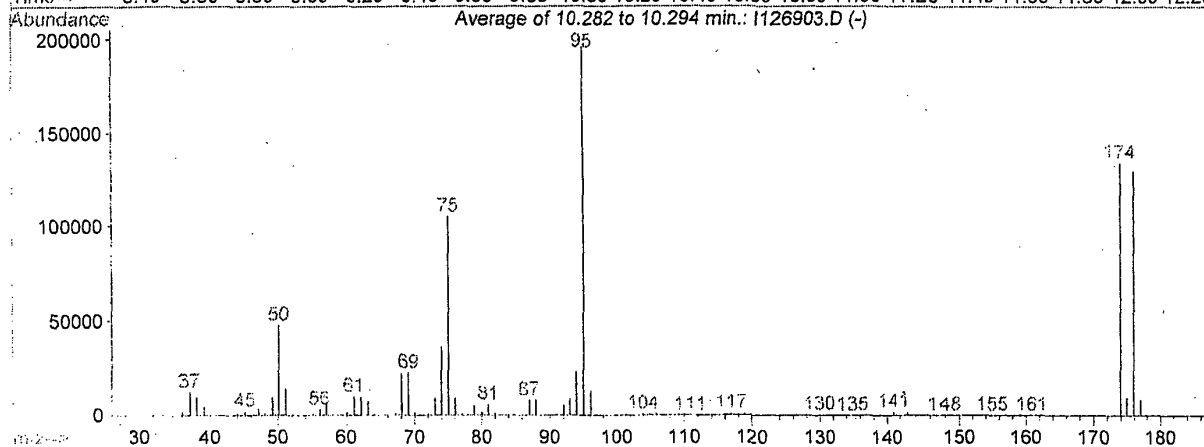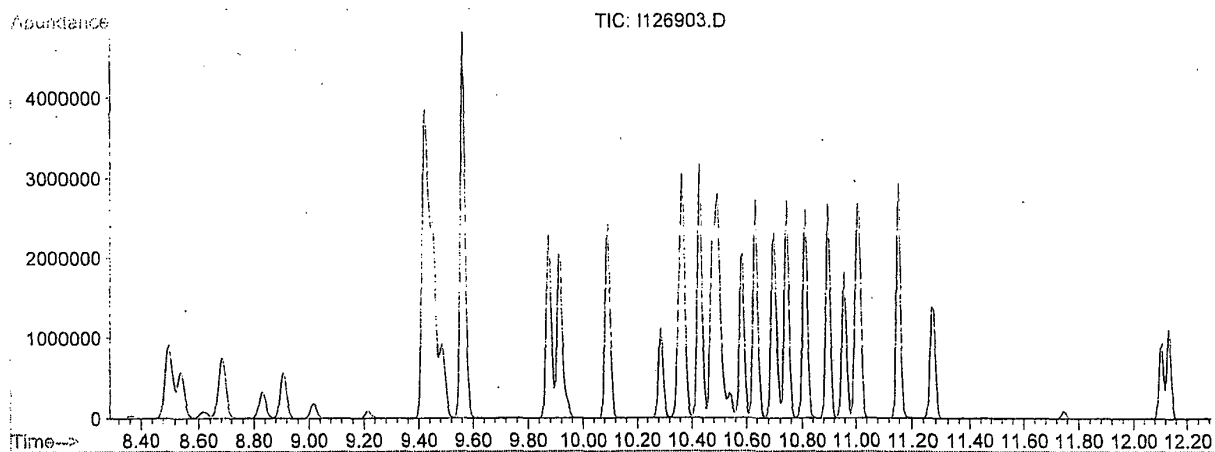

AutoFind: Scans 1511, 1512, 1513; Background Corrected with Scan 1505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	47832	PASS
75	95	30	60	53.8	105237	PASS
95	95	100	100	100.0	195627	PASS
96	95	5	9	6.8	13301	PASS
173	174	0.00	2	0.4	591	PASS
174	95	50	100	68.8	134555	PASS
175	174	5	9	7.1	9592	PASS
176	174	95	101	96.6	130029	PASS
177	176	5	9	6.5	8430	PASS

WMT
1/20/09

Injection Log

7 / 132

Directory: h:\msi\i\012609.b

PS

JAN 27 2009

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	1	i126901.d	1.	BLANK	1,1, 9010001 5uL/50mL	26 Jan 09 05:31
2	2	i126902.d	1.	BLANK	1,1, 9010225 5uL/50mL	26 Jan 09 05:59
3	3	i126903.d	1.	CCV,REGC	9010191 5uL/50mL	26 Jan 09 06:26
4	4	i126904.d	1.	BATCH-BS1@1,REGC	9010191 5uL/50mL	26 Jan 09 06:53
5	5	i126905.d	1.	BATCH-BSD1@1,REGC	9010191 5uL/50mL	26 Jan 09 07:20
6	6	i126906.d	1.	BATCH-MS1@1X MS,REGC	9010191 4.2uL/42mL; VIALS 1-J,M,Q;G	26 Jan 09 08:21
7	7	i126907.d	1.	BATCH-MSD1@1X MSD,REGC	9010191 4.2uL/42mL; VIALS 1-J,M,Q;G	26 Jan 09 08:48
8	8	i126908.d	1.	CCV,REG	9010191 5uL/50mL	26 Jan 09 09:15
9	9	i126909.d	1.	BLANK	1,1, 9010225 5uL/50mL	26 Jan 09 09:43
10	10	i126910.d	1.	BLANK	1,1, 9010225 5uL/50mL	26 Jan 09 10:10
11	11	i126911.d	1.	BATCH-BLK1@1,REGC	1,1, 9010225 5uL/50mL	26 Jan 09 10:37
12	12	i126912.d	1.	ASA0148-01 0@1X ,REGC	VIALS 1-J,M,Q;G	26 Jan 09 11:04
13	13	i126913.d	1.	ASA0086-01 @1X A,REGC		26 Jan 09 11:32
14	14	i126914.d	1.	ASA0086-02 @1X A,REGC		26 Jan 09 11:59
15	15	i126915.d	1.	ASA0086-03 @1X A,REGC		26 Jan 09 12:26
16	16	i126916.d	1.	ASA0122-12 @1X C,53765		26 Jan 09 12:53
17	17	i126917.d	1.	ASA0156-02 @1X A,BTEX		26 Jan 09 13:21
18	18	i126918.d	1.	ASA0156-01 @100X A,BTEX		26 Jan 09 13:48
19	19	i126919.d	1.	ASA0122-13 @1X C,53765		26 Jan 09 14:15
20	20	i126920.d	1.	ASA0122-14 @1X C,53765		26 Jan 09 14:43
21	21	i126921.d	1.	ASA0122-15 @1X C,53765		26 Jan 09 15:10
22	22	i126922.d	1.	ASA0122-16 @1X E,53765		26 Jan 09 15:38
23	23	i126923.d	1.	ASA0122-17 @1X C,53765		26 Jan 09 16:05
24	24	i126924.d	1.	ASA0122-18 @1X D,53765		26 Jan 09 16:37
25	25	i126925.d	1.	ASA0122-19 @1X B,53765		26 Jan 09 17:05
26	26	i126926.d	1.	ASA0131-07 @1X A,57989		26 Jan 09 17:33
27	27	i126927.d	1.	ASA0131-08 @1X A,57989		26 Jan 09 18:00
28	28	i126928.d	1.	ASA0131-09 @1X A,57989		26 Jan 09 18:28
29	29	i126929.d	1.	ASA0131-10 @1X A,57989		26 Jan 09 18:55
30	30	i126930.d	1.	ASA0131-11 @1X A,57989		26 Jan 09 19:23
31	31	i126931.d	1.	ASA0131-12 @1X A,57989		26 Jan 09 19:50
32	32	i126932.d	1.	ASA0086-01RE1 @2X A,CIS	CIS-D	26 Jan 09 20:17

BFB

Data File : H:\MSI.I\I012609.B\I126908.D

Acq On : 26 Jan 2009 9:15 am

Sample : CCV,REG

Misc : 9010191 5uL/50mL

MS Integration Params: VOA.P

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)



Title : EPA Method 8260B/624 Calibration Curve 15mL Water

Vial: 8

Operator: DY

Inst : MSI

Multiplr: 1.00

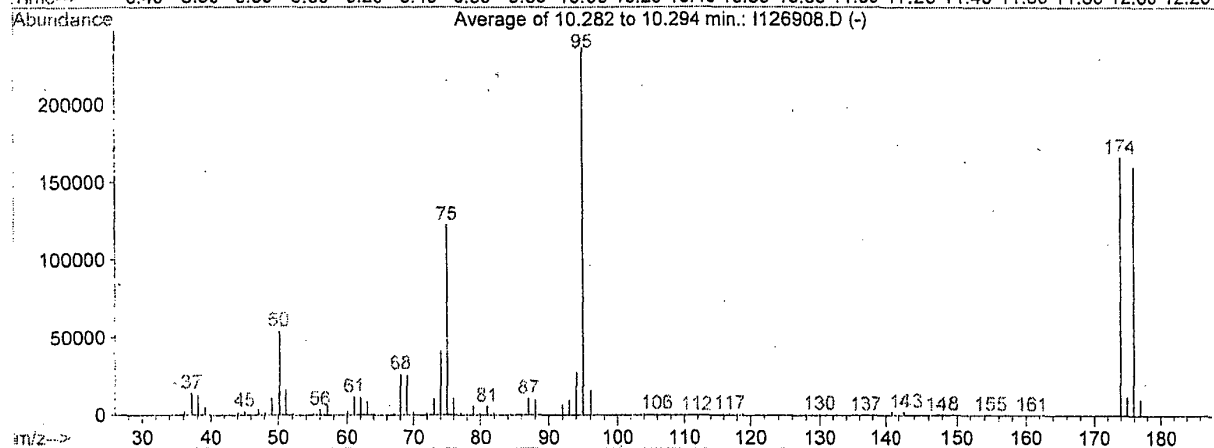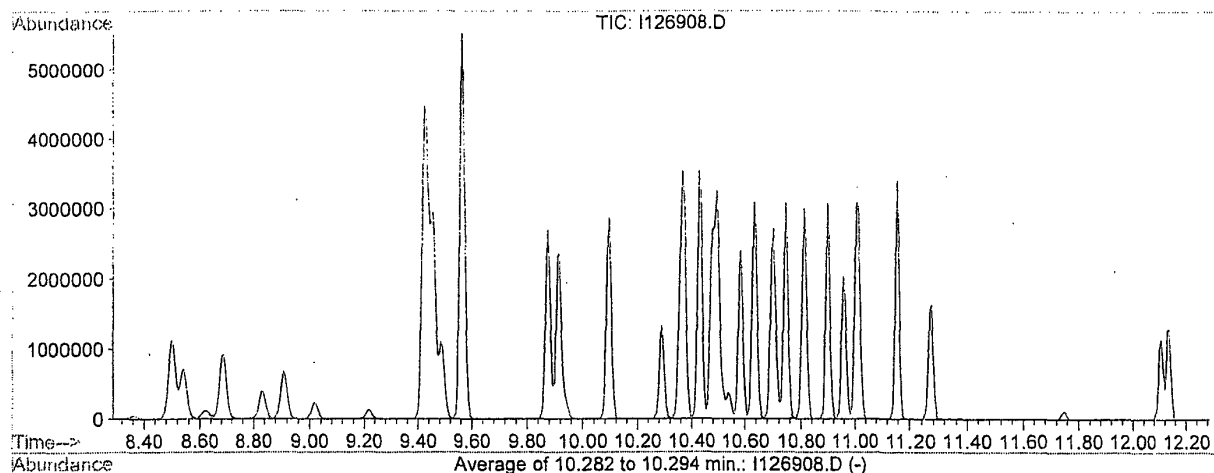

AutoFind: Scans 1511, 1512, 1513; Background Corrected with Scan 1505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	54027	PASS
75	95	30	60	51.8	122221	PASS
95	95	100	100	100.0	235819	PASS
96	95	5	9	6.8	15953	PASS
173	174	0.00	2	0.2	360	PASS
174	95	50	100	70.5	166221	PASS
175	174	5	9	7.0	11654	PASS
176	174	95	101	96.4	160245	PASS
177	176	5	9	6.4	10335	PASS

Boh 11/7/08

Calibration Table Report													
Method: I81104W.M													
Title: EPA Method 8260B/624 Calibration Curve 15mL Water													
Last Calibration: Fri Nov 07 15:27:57 2008													
Calibration Files	0.5	1	2	5	10	20	50	100					
	IB04805.D	IB04806.D	IB04807.D	IB04808.D	IB04809.D	IB04810.D	IB04811.D	IB04812.D					
Compound									Avg	%RSD	LR	QR	
										≤15%	≥0.990	≥0.990	
Fluorobenzene (IS)	ISTD												
Dichlorodifluoromethane	0.441	0.388	0.347	0.374	0.368	0.362	0.353	0.320	0.369	9.558			
Chloromethane (SPCC)	0.392	0.363	0.333	0.369	0.347	0.358	0.366	0.367	0.362	4.768			
Vinyl chloride (CCC)	0.446	0.408	0.355	0.386	0.384	0.388	0.391	0.372	0.391	6.805			
Bromomethane	✓	0.252	0.207	0.192	0.174	0.180	0.201	0.222	0.204	13.025			
Ethylene oxide	✓	0.034	0.030	0.030	0.028	0.027			0.030	9.288			
Chloroethane	0.309	0.292	0.262	0.264	0.264	0.263	0.255	0.205	0.264	11.403			
Trichlorofluoromethane	0.494	0.430	0.384	0.405	0.397	0.392	0.387	0.354	0.405	10.221			
Ethyl ether	0.227	0.211	0.202	0.203	0.206	0.208	0.205	0.199	0.208	4.205			
Ethanol	✓	0.001	0.001	0.001	0.001	0.001	0.002	0.001	0.001	6.316			
1,1-Dichloroethene (CCC)	0.286	0.256	0.226	0.241	0.242	0.248	0.253	0.250	0.250	6.897			
Carbon disulfide	0.964	0.846	0.797	0.843	0.871	0.896	0.924	0.906	0.881	5.986			
1,1,2-Trichlorotrifluoroethane	0.289	0.261	0.224	0.237	0.233	0.234	0.234	0.219	0.242	9.442			
Propylene oxide	0.029	0.029	0.027	0.029	0.031	0.031	0.031	0.029	0.030	4.312			
Iodomethane	✓	0.139	0.173	0.261	0.338	0.375	0.388	0.387	0.294	35.546	1.000		
Bromoethane	0.222	0.205	0.197	0.194	0.200	0.202	0.202	0.205	0.203	4.101			
Acrolein	0.013	0.013	0.013	0.014	0.015	0.015	0.016	0.016	0.014	8.790			
3-Chloropropene	0.535	0.489	0.483	0.503	0.516	0.523	0.517	0.496	0.508	3.539			
Methylene chloride	0.329	0.301	0.275	0.276	0.279	0.278	0.277	0.273	0.286	6.845			
Acetone	✓	0.011	0.012	0.011	0.013	0.013	0.013	0.013	0.012	6.517			
trans-1,2-Dichloroethene	0.320	0.277	0.264	0.272	0.275	0.278	0.280	0.283	0.281	5.905			
Methyl acetate	0.021	0.021	0.020	0.022	0.022	0.022	0.022	0.022	0.021	4.343			
Hexane	0.107	0.094	0.086	0.092	0.093	0.094	0.095	0.088	0.094	6.806			
Methyl tert-butyl ether (MTBE)	0.606	0.596	0.558	0.572	0.590	0.590	0.589	0.569	0.584	2.743			
tert-Butyl alcohol	0.010	0.011	0.011	0.010	0.012	0.012	0.013	0.012	0.011	8.127			
Acetonitrile	0.012	0.010	0.010	0.010	0.010	0.010	0.010	0.009	0.010	6.460			
Isopropyl ether	1.085	1.034	0.993	1.021	1.051	1.059	1.034	0.979	1.032	3.333			
2-Chloro-1,3-butadiene	0.214	0.194	0.185	0.209	0.222	0.233	0.238	0.237	0.217	9.134			


Calibration Files	0.5	1	2	5	10	20	50	100				
	IB04805.D	IB04806.D	IB04807.D	IB04808.D	IB04809.D	IB04810.D	IB04811.D	IB04812.D				
Compound									Avg	%RSD	LR	QR
										≤15%	≥0.990	≥0.990
1,1-Dichloroethane (SPCC)	0.616	0.567	0.534	0.536	0.546	0.546	0.536	0.523	0.551	5.316		
Acrylonitrile	0.054	0.053	0.050	0.052	0.054	0.053	0.053	0.052	0.053	2.661		
Vinyl acetate	0.302	0.291	0.304	0.326	0.355	0.365	0.368	0.354	0.333	9.333		
cis-1,2-Dichloroethene	0.323	0.291	0.283	0.284	0.293	0.295	0.300	0.301	0.296	4.186		
2,2-Dichloropropane	0.443	0.423	0.386	0.406	0.413	0.419	0.413	0.401	0.413	4.074		
Cyclohexane	0.594	0.521	0.472	0.515	0.513	0.509	0.509	0.470	0.513	7.458		
Bromochloromethane	0.147	0.140	0.130	0.131	0.136	0.140	0.141	0.144	0.139	4.251		
2-Methylhexane (NC)												
Chloroform (CCC)	0.524	0.488	0.461	0.467	0.469	0.468	0.466	0.460	0.475	4.498		
Carbon tetrachloride	0.353	0.322	0.290	0.319	0.326	0.326	0.323	0.314	0.322	5.390		
3-Methylhexane (NC)												
Ethyl acetate	0.134	0.130	0.127	0.131	0.139	0.138	0.136	0.128	0.133	3.447		
Tetrahydrofuran			0.017	0.017	0.020	0.020	0.021	0.020	0.019	8.500		
Dibromofluoromethane (Surr)	0.253	0.242	0.228	0.234	0.244	0.246	0.249	0.251	0.244	3.584		
1,1,1-Trichloroethane	0.438	0.401	0.369	0.395	0.396	0.396	0.399	0.388	0.398	4.782		
1,1-Dichloropropene	0.413	0.376	0.351	0.377	0.387	0.387	0.388	0.378	0.382	4.573		
2-Butanone (MEK)	0.071	0.070	0.052	0.054	0.058	0.060	0.061	0.059	0.060	11.154		
Benzene	1.323	1.211	1.149	1.168	1.194	1.208	1.201	1.180	1.204	4.360		
Heptane (NC)												
Propanenitrile	0.018	0.019	0.019	0.020	0.020	0.020	0.021	0.020	0.020	4.419		
Methacrylonitrile	0.061	0.058	0.058	0.063	0.067	0.067	0.068	0.066	0.063	6.629		
1,2-Dichloroethane-d4 (Surr)	0.167	0.156	0.140	0.133	0.133	0.132	0.127	0.124	0.139	10.694		
1,2-Dichloroethane	0.334	0.306	0.291	0.281	0.291	0.282	0.275	0.265	0.291	7.306		
Isobutyl alcohol	0.004	0.004	0.004	0.005	0.005	0.006	0.006	0.006	0.005	17.006	0.999	
Methylcyclohexane	0.412	0.372	0.331	0.356	0.358	0.358	0.366	0.343	0.362	6.641		
Trichloroethene	0.317	0.276	0.264	0.264	0.269	0.274	0.281	0.288	0.279	6.240		
Dibromomethane	0.112	0.102	0.098	0.100	0.106	0.107	0.107	0.107	0.105	4.344		
n-Butanol	0.002	0.002	0.002	0.002	0.003	0.004	0.004	0.004	0.003	29.253	0.999	
1,2-Dichloropropane (CCC)	0.311	0.280	0.267	0.271	0.282	0.282	0.281	0.279	0.282	4.609		
Bromodichloromethane	0.334	0.306	0.297	0.313	0.331	0.331	0.335	0.338	0.323	4.821		
1,4-Dioxane	0.001	0.001	0.001	0.001	0.001	0.001	0.001	0.001	0.001	12.800		
Methyl methacrylate	0.079	0.072	0.080	0.089	0.102	0.109	0.116	0.116	0.095	18.534	1.000	
1-Bromo-2-chloroethane	0.320	0.304	0.283	0.281	0.297	0.299	0.300	0.297	0.298	4.061		
cis-1,3-Dichloropropene	0.373	0.359	0.362	0.381	0.418	0.428	0.434	0.431	0.398	8.196		

Calibration Files	0.5	1	2	5	10	20	50	100				
	IB04805.D	IB04806.D	IB04807.D	IB04808.D	IB04809.D	IB04810.D	IB04811.D	IB04812.D				
Compound									Avg	%RSD	LR	QR
										≤15%	≥0.990	≥0.990
1-Chloroethyl vinyl ether	✓	✓	0.070	0.076	0.087	0.090	0.092	0.088	0.084	10.583		
Toluene-d8 (Surr)	0.985	0.936	0.892	0.920	0.964	0.983	0.997	0.993	0.959	4.022		
Chlorobenzene-d5 (IS)	ISTD											
Toluene (CCC)	6.128	5.837	5.563	5.599	5.668	5.672	5.395	5.240	5.638	4.769		
1,2-Dichloroethane	0.056	0.051	0.054	0.057	0.061	0.062	0.061	0.057	0.057	6.453		
2-Nitropropane	✓	✓	✓	0.114	0.130	0.146	0.157	0.161	0.142	13.697		
Tetrachloroethene	1.107	0.964	0.865	0.909	0.916	0.907	0.900	0.896	0.933	8.078		
4-Methyl-2-pentanone (MIBK)	0.496	0.501	0.529	0.559	0.612	0.639	0.626	0.586	0.569	9.857		
trans-1,3-Dichloropropene	1.335	1.306	1.365	1.449	1.575	1.594	1.518	1.478	1.452	7.483		
1,1,2-Trichloroethane	0.789	0.787	0.775	0.774	0.787	0.771	0.738	0.728	0.769	2.982		
4-Methyl-2-pentanol (MIBC)	✓	0.066	0.073	0.080	0.098	0.110	0.133	0.132	0.099	27.716	0.999	
Ethyl methacrylate	✓	0.683	0.770	0.862	1.024	1.087	1.096	1.070	0.942	17.932	1.000	
Dibromochloromethane	0.790	0.763	0.755	0.810	0.867	0.898	0.875	0.874	0.829	6.777		
1,3-Dichloropropane	1.792	1.628	1.559	1.544	1.575	1.540	1.448	1.406	1.562	7.501		
1,2-Dibromoethane (EDB)	0.717	0.675	0.652	0.670	0.699	0.688	0.677	0.658	0.680	3.154		
2-Hexanone	✓	0.294	0.341	0.373	0.379	0.398	0.384	0.658	0.349	13.380		
Chlorobenzene (SPCC)	4.063	3.634	3.357	3.337	3.351	3.370	3.354	3.328	3.474	7.432		
1-Chlorohexane	2.543	1.872	1.475	1.414	1.341	1.307	1.207	1.102	1.533	30.526		1.000
Ethylbenzene (CCC)	2.240	1.980	1.834	1.895	1.960	1.971	1.938	1.943	1.970	6.034		
1,1,1,2-Tetrachloroethane	1.089	1.069	1.005	1.036	1.083	1.086	1.068	1.071	1.063	2.699		
m&p-Xylene	2.617	2.431	2.299	2.369	2.462	2.468	2.475	2.408	2.441	3.794		
o-Xylene	2.318	2.207	2.099	2.196	2.328	2.333	2.311	2.303	2.262	3.753		
Bromoform (SPCC)	0.328	0.320	0.325	0.350	0.393	0.405	0.419	0.425	0.371	12.053		
Styrene	2.870	2.782	2.894	3.347	3.660	3.759	3.756	3.734	3.350	13.043		
Isopropylbenzene	5.543	5.274	5.038	5.347	5.450	5.485	5.328	5.180	5.331	3.132		
Bromobenzene	1.178	1.092	1.083	1.100	1.143	1.139	1.153	1.185	1.134	3.412		
n-Propylbenzene	1.477	1.421	1.412	1.500	1.554	1.552	1.578	1.593	1.511	4.607		
1,1,1,2-Tetrachloroethane (SPCC)	0.835	0.823	0.781	0.780	0.801	0.795	0.788	0.773	0.797	2.739		
1,4-Bromofluorobenzene (Surr)	1.702	1.601	1.511	1.523	1.563	1.576	1.516	1.497	1.561	4.314		
1,4-Dichlorobenzene-d4 (IS)	ISTD											
2-Chlorotoluene	1.043	0.978	0.910	0.941	0.965	0.968	0.983	0.973	0.970	3.922		
Cyclohexanone	✓	✓	0.009	0.009	0.010	0.009	0.011	0.010	0.010	7.259		
1,2,3-Trichloropropane	0.222	0.211	0.202	0.197	0.198	0.194	0.193	0.185	0.200	5.817		
trans-1,4-Dichloro-2-butene	✓	0.116	0.125	0.137	0.157	0.163	0.173	0.165	0.148	14.834		

Calibration Files	0.5	1	2	5	10	20	50	100				
	IB04805.D	IB04806.D	IB04807.D	IB04808.D	IB04809.D	IB04810.D	IB04811.D	IB04812.D				
Compound									Avg	%RSD	LR	QR
										≤15%	≥0.990	≥0.990
-Ethyltoluene	4.196	4.007	3.905	4.103	4.262	4.254	4.264	4.038	4.129	3.304		
-Chlorotoluene	1.027	0.945	0.911	0.931	0.965	0.977	0.975	0.962	0.962	3.610		
,3,5-Trimethylbenzene	3.600	3.445	3.300	3.467	3.562	3.592	3.539	3.390	3.487	3.041		
-Ethyltoluene	4.365	4.202	4.032	4.131	4.289	4.270	4.199	3.991	4.185	3.060		
ert-Butylbenzene	2.107	1.974	1.854	1.910	1.926	1.914	1.859	1.765	1.914	5.217		
pentachloroethane	0.428	0.413	0.442	0.459	0.503	0.534	0.551	0.567	0.487	12.216		
,2,4-Trimethylbenzene	3.486	3.476	3.340	3.441	3.594	3.616	3.575	3.406	3.492	2.783		
ec-Butylbenzene	4.697	4.321	4.041	4.179	4.281	4.286	4.264	4.005	4.259	4.985		
-Isopropyltoluene	3.688	3.555	3.407	3.595	3.740	3.763	3.772	3.599	3.640	3.449		
1,3-Dichlorobenzene	1.938	1.757	1.656	1.636	1.690	1.710	1.724	1.712	1.728	5.396		
1,4-Dichlorobenzene	2.125	1.908	1.769	1.726	1.775	1.761	1.799	1.770	1.829	7.153		
benzyl chloride	✓	✓	0.102	0.139	0.169	0.204	0.242	0.261	0.186	32.922	0.999	
-Butylbenzene	0.862	0.784	0.734	0.818	0.871	0.893	0.917	0.917	0.850	7.745		
1,2-Dichlorobenzene	1.568	1.459	1.355	1.371	1.434	1.445	1.436	1.428	1.437	4.459		
1,3,5-Trichlorobenzene (NC)												
1,2-Dibromo-3-chloropropane (DBCP)	✓	0.049	0.052	0.059	0.066	0.073	0.086	0.084	0.067	21.793	0.999	
Hexachlorobutadiene	0.486	0.467	0.411	0.413	0.417	0.421	0.438	0.435	0.436	6.217		
1,2,4-Trichlorobenzene	0.763	0.758	0.694	0.732	0.780	0.801	0.812	0.799	0.767	5.190		
Naphthalene	0.898	0.954	0.984	1.070	1.208	1.273	1.305	1.237	1.116	14.253		
1,2,3-Trichlorobenzene	0.552	0.551	0.526	0.522	0.552	0.554	0.559	0.544	0.545	2.483		

Fri Nov 07 15:34:57 2008

8260 WATER CALCHECK (FORM VII)-- SOP LIMITS

 JAN 27 2009

I126903.D		SPCC											
COMPOUND	SPIKE (ug/L)	AVG RF	AC	CCV RF	RF TOL	> OR =	P/F	%DIFFERENCE	CC REC	CCC REC TOL			
								RESULT TOL (%) P/F	%	LOW	HIGH	P/F	
Fluorobenzene (IS)	16.7	44192.403	735048	1.000					0				
Dichlorodifluoromethane	20	0.369	342764	0.389				5.51	106	50	150		
Chloromethane (SPCC)	20	0.362	314569	0.357	0.10			-1.25	99	50	150		
Vinyl chloride (CCC)	20	0.391	387036	0.440				12.38 20	112				
Bromomethane	20	0.204	191262	0.217				6.50	106	50	150		
Ethylene oxide	250	0.030	319165	0.029				-2.65	97	10	200		
Chloroethane	20	0.264	260439	0.296				11.94	112	50	150		
Trichlorofluoromethane	20	0.405	421060	0.478				17.97	118	50	150		
Ethyl ether	20	0.208	164036	0.186				-10.25	90	50	150		
Ethanol	500	0.001	0	0.000				-100.00	0				
1,1-Dichloroethene (CCC)	20	0.250	218354	0.248				-0.96 20	99				
Carbon disulfide	20	0.881	850581	0.966				9.68	110	50	150		
1,1,2-Trichlorotrifluoroethane	20	0.242	241798	0.275				13.74	114	50	150		
Propylene oxide	100	0.030	108710	0.025				-16.44	84	10	200		
Iodomethane	20	0.392	286430	0.325				-16.99	83	65	135		
Bromoethane	20	0.203	172766	0.196				-3.47	97	65	135		
Acrolein	100	0.014	73560	0.017				16.48	116	10	200		
3-Chloropropene	20	0.508	548080	0.623				22.63	123	65	135		
Methylene chloride	20	0.286	225172	0.256				-10.59	89	65	135		
Acetone	20	0.012	8191	0.009				-24.68	75	50	150		
trans-1,2-Dichloroethene	20	0.281	252376	0.287				2.02	102	65	135		
Methyl acetate	50	0.021	39984	0.018				-15.20	85	50	150		
Hexane	20	0.094	94487	0.107				14.53	115	65	135		
Methyl tert-butyl ether (MTBE)	20	0.584	435267	0.494				-15.31	85	65	135		
tert-Butyl alcohol	500	0.011	148349	0.007				-40.58	59	10	200		
Acetonitrile	100	0.010	37755	0.009				-15.04	85	50	150		
Isopropyl ether	20	1.032	1000289	1.136				10.09	110	65	135		
2-Chloro-1,3-butadiene	20	0.217	210291	0.239				-10.30	110	65	135		
1,1-Dichloroethane (SPCC)	20	0.551	528534	0.600	0.10			9.04	109	65	135		
Acrylonitrile	100	0.053	202976	0.046				-12.16	88	50	150		
Vinyl acetate	20	0.333	314631	0.357				7.31	107	10	200		
cis-1,2-Dichloroethene	20	0.296	248121	0.282				-4.84	95	65	135		
2,2-Dichloropropane	20	0.413	379875	0.432				4.51	105	65	135		
Cyclohexane	20	0.513	582817	0.662				29.11	129	65	135		
Bromochloromethane	20	0.139	106434	0.121				-12.84	87	65	135		
2-Methylhexane (NC)	20	0.000	0	0.000				NC		50	150		
Chloroform (CCC)	20	0.475	408618	0.464				-2.37 20	98				
Carbon tetrachloride	20	0.322	325905	0.370				15.12	115	65	135		
3-Methylhexane (NC)	20	0.000	0	0.000				NC		50	150		
Ethyl acetate	100	0.133	0	0.000				-100.00	0	50	150		
Tetrahydrofuran	20	0.019	15291	0.017				-9.67	90	50	150		
1,1,1-Trichloroethane	20	0.398	381066	0.433				8.88	109	65	135		
1,1-Dichloropropene	20	0.382	392776	0.446				16.75	117	65	135		
2-Butanone (MEK)	20	0.060	44822	0.051				-15.77	84	50	150		
Benzene	20	1.204	1127348	1.281				6.35	106	65	135		
Heptane (NC)	20	0.000	0	0.000				NC		50	150		
Propanenitrile	100	0.020	76498	0.017				-11.92	88	50	150		
Methacrylonitrile	100	0.063	253591	0.058				-9.17	91	50	150		
1,2-Dichloroethane	20	0.291	280129	0.318				9.53	110	65	135		
Isobutyl alcohol	500	0.006	71610	0.003				-47.40	53	50	150		
Methylcyclohexane	50	0.362	979301	0.445				22.97	123	50	150		

8260 WATER CALCHECK (FORM VII)-- SOP LIMITS

1126903.D					SPCC										
COMPOUND	SPIKE (ug/L)	AVG RF	AC	CCV RF	RF TOL	> OR =	P/F	RESULT	TOL (%)	P/F	CC REC %	CCC REC TOL	LOW	HIGH	P/F
Trichloroethene	20	0.279	248108	0.282				0.99			101	65	135		
Dibromomethane	20	0.105	87423	0.099				-5.24			95	65	135		
n-Butanol	1000	0.004	75775	0.002				-58.10			42	10	200		
1,2-Dichloropropane (CCC)	20	0.282	265264	0.301				6.96	20		107				
Bromodichloromethane	20	0.323	291297	0.331				2.39			102	65	135		
1,4-Dioxane	500	0.001	17214	0.001				-37.79			62	10	200		
Methyl methacrylate	20	0.117	73145	0.083				-28.91			71	50	150		
1-Bromo-2-chloroethane	20	0.298	252379	0.287				-3.67			96	65	135		
cis-1,3-Dichloropropene	20	0.398	368092	0.418				5.02			105	65	135		
2-Chloroethyl vinyl ether	20	0.084	67143	0.076				-9.07			91	10	200		
Chlorobenzene-d5 (IS)	16.7	1.000	173796	1.000							100				
Toluene (CCC)	20	5.638	1141941	5.486				-2.68	20		97				
Epichlorohydrin	100	0.057	46452	0.045				-22.32			78	50	150		
2-Nitropropane	20	0.142	24327	0.117				-17.45			83	10	200		
Tetrachloroethene	20	0.933	171622	0.825				-11.62			88	65	135		
4-Methyl-2-pentanone (MIBK)	20	0.569	108058	0.519				-8.68			91	50	150		
trans-1,3-Dichloropropene	20	1.452	279003	1.340				-7.71			92	65	135		
1,1,2-Trichloroethane	20	0.769	132309	0.636				-17.30			83	65	135		
4-Methyl-2-pentanol (MIBC)	100	0.135	56670	0.054				-59.53			40	50	150		
Ethyl methacrylate	20	1.081	172381	0.828				-23.36			77	50	150		
Dibromochloromethane	20	0.829	150933	0.725				-12.53			87	65	135		
1,3-Dichloropropane	20	1.562	281224	1.351				-13.47			87	65	135		
1,2-Dibromoethane (EDB)	20	0.680	116646	0.560				-17.53			82	65	135		
2-Hexanone	20	0.349	58796	0.282				-19.16			81	50	150		
Chlorobenzene (SPCC)	20	3.474	707342	3.398	0.30			-2.18			98	65	135		
1-Chlorohexane	20	1.303	341612	1.641				25.96			126	65	135		
Ethylbenzene (CCC)	20	1.970	412996	1.984				0.72	20		101				
1,1,1,2-Tetrachloroethane	20	1.063	209565	1.007				-5.31			95	65	135		
m&p-Xylene	40	2.441	1053312	2.530				3.65			104	65	135		
o-Xylene	20	2.262	483716	2.324				2.75			103	65	135		
Bromoform (SPCC)	20	0.371	70531	0.339	0.10			-8.57			91	50	150		
Styrene	20	3.350	752607	3.616				7.93			108	65	135		
Isopropylbenzene	20	5.331	1257770	6.043				13.36			113	65	135		
Bromobenzene	20	1.134	231316	1.111				-2.00			98	65	135		
n-Propylbenzene	20	1.511	318423	1.530				1.27			101	65	135		
1,1,2,2-Tetrachloroethane (SPCC)	20	0.797	153311	0.737	0.30			-7.58			92	65	135		
1,4-Dichlorobenzene-d4 (IS)	16.7	1.000	244344	1.000							100				
2-Chlorotoluene	20	0.970	287170	0.981				1.17			101	65	135		
Cyclohexanone	100	0.010	0	0.000				-100.00			0				
1,2,3-Trichloropropane	20	0.200	45226	0.155				-22.79			77	65	135		
trans-1,4-Dichloro-2-butene	20	0.148	46665	0.159				7.58			108	50	150		
3-Ethyltoluene	20	4.129	1257078	4.296				4.05			104	65	135		
4-Chlorotoluene	20	0.962	281280	0.961				-0.05			100	65	135		
1,3,5-Trimethylbenzene	20	3.487	1029437	3.518				0.89			101	65	135		
2-Ethyltoluene	20	4.185	1242385	4.246				1.45			101	65	135		

8260 WATER CALCHECK (FORM VII)-- SOP LIMITS

I126903.D		SPCC					%DIFFERENCE			CC REC			CCC REC.TOL		
COMPOUND	SPIKE (ug/L)	AVG RF	AC	CCV RF	RF TOL	> OR =	P/F	RESULT	TOL (%)	P/F	%	LOW	HIGH	P/F	
tert-Butylbenzene	20	1.914	589290	2.014				5.23			105	65	135		
Pentachloroethane	50	0.487	0	0.000				100.00			20	50	150	Q	
1,2,4-Trimethylbenzene	20	3.492	1032432	3.528				1.04			101	65	135		
sec-Butylbenzene	20	4.259	1357879	4.640				8.95			109	65	135		
p-Isopropyltoluene	20	3.640	1087220	3.715				2.07			102	65	135		
1,3-Dichlorobenzene	20	1.728	486992	1.664				-3.69			96	65	135		
1,4-Dichlorobenzene	20	1.829	498042	1.702				-6.96			93	65	135		
Benzyl chloride	20	0.267	42836	0.146				-45.11			55	10	200		
n-Butylbenzene	20	0.850	248596	0.850				-0.02			100	65	135		
1,2-Dichlorobenzene	20	1.437	391594	1.338				-6.88			93	65	135		
1,3,5-Trichlorobenzene (NC)	50	0.000	0	0.000				NC				65	135		
1,2-Dibromo-3-chloropropane (DBC)	20	0.086	13474	0.046				-46.22			54	50	150		
Hexachlorobutadiene	20	0.436	117805	0.403				-7.67			92	50	150		
1,2,4-Trichlorobenzene	20	0.767	223244	0.763				-0.60			99	50	150		
Naphthalene	20	1.116	316662	1.082				-3.03			97	50	150		
1,2,3-Trichlorobenzene	20	0.545	145859	0.498				-8.54			91	50	150		
Dibromofluoromethane (Surr)	16.7	0.244	179787	0.245				0.42			100	84	116		
1,2-Dichloroethane-d4 (Surr)	16.7	0.139	103893	0.141				1.71			102	73	126		
Toluene-d8 (Surr)	16.7	0.959	797148	1.084				13.10			113	89	119		
1,4-Bromofluorobenzene (Surr)	16.7	1.561	285176	1.641				5.12			105	80	116		

NT

Q - Failed criteria
 NC-Not Calibrated

8260 WATER CALCHECK (FORM VII)-- SOP LIMITS

JAN 27 2009

I126908.D					SPCC		%DIFFERENCE		CC REC		CCC REC TOL			
COMPOUND	SPIKE (ug/L)	AVG RF	AC	CCV RF	RF TOL	> OR =	P/F	RESULT	TOL (%)	P/F	%	LOW	HIGH	P/F
Fluorobenzene (IS)	16.7	44192.403	924953	1.000							0			
Dichlorodifluoromethane	20	0.369	402734	0.364				-1.49			99	50	150	
Chloromethane (SPCC)	20	0.362	443172	0.400	0.10			10.56			111	50	150	
Vinyl chloride (CCC)	20	0.391	482697	0.436				11.38	20		111			
Bromomethane	20	0.204	267810	0.242				18.50			119	50	150	
Ethylene oxide	250	0.030	395624	0.029				-4.10			96	10	200	
Chloroethane	20	0.264	319861	0.289				9.26			109	50	150	
Trichlorofluoromethane	20	0.405	499976	0.451				11.32			111	50	150	
Ethyl ether	20	0.208	220867	0.199				-3.96			96	50	150	
Ethanol	500	0.001	0	0.000				-100.00			0			
1,1-Dichloroethene (CCC)	20	0.250	282209	0.255				1.72	20		102			
Carbon disulfide	20	0.881	1076929	0.972				10.36			110	50	150	
1,1,2-Trichlorotrifluoroethane	20	0.242	299960	0.271				12.13			112	50	150	
Propylene oxide	100	0.030	148211	0.027				-9.47			91	10	200	
Iodomethane	20	0.392	352611	0.318				-18.79			81	65	135	
Bromoethane	20	0.203	222853	0.201				-1.05			99	65	135	
Acrolein	100	0.014	104251	0.019				31.19			131	10	200	
3-Chloropropene	20	0.508	670219	0.605				19.17			119	65	135	
Methylene chloride	20	0.286	290454	0.262				-8.35			92	65	135	
Acetone	20	0.012	12258	0.011				-10.42			90	50	150	
trans-1,2-Dichloroethene	20	0.281	327479	0.296				5.20			105	65	135	
Methyl acetate	50	0.021	59108	0.021				-0.37			100	50	150	
Hexane	20	0.094	118222	0.107				13.88			114	65	135	
Methyl tert-butyl ether (MTBE)	20	0.584	603998	0.545				-6.61			93	65	135	
tert-Butyl alcohol	500	0.011	249372	0.009				-20.63			79	10	200	
Acetonitrile	100	0.010	49870	0.009				-10.82			89	50	150	
Isopropyl ether	20	1.032	1272913	1.149				11.33			111	65	135	
2-Chloro-1,3-butadiene	20	0.217	269091	0.243				12.16			112	65	135	
1,1-Dichloroethane (SPCC)	20	0.551	643479	0.581	0.10			5.50			105	65	135	
Acrylonitrile	100	0.053	276908	0.050				-4.77			95	50	150	
Vinyl acetate	20	0.333	431725	0.390				17.02			117	10	200	
cis-1,2-Dichloroethene	20	0.296	322236	0.291				-1.79			98	65	135	
2,2-Dichloropropane	20	0.413	472690	0.427				3.35			103	65	135	
Cyclohexane	20	0.513	700689	0.633				23.35			123	65	135	
Bromochloromethane	20	0.139	142190	0.128				-7.47			93	65	135	
2-Methylhexane (NC)	20	0.000	0	0.000				NC				50	150	
Chloroform (CCC)	20	0.475	510946	0.461				-2.98	20		97			
Carbon tetrachloride	20	0.322	397911	0.359				11.69			112	65	135	
3-Methylhexane (NC)	20	0.000	0	0.000				NC				50	150	
Ethyl acetate	100	0.133	0	0.000				100.00			0	50	150	
Tetrahydrofuran	20	0.019	20822	0.019				-2.25			98	50	150	
1,1,1-Trichloroethane	20	0.398	466055	0.421				5.82			106	65	135	
1,1-Dichloropropene	20	0.382	482618	0.436				14.00			114	65	135	
2-Butanone (MEK)	20	0.060	64735	0.058				-3.33			97	50	150	
Benzene	20	1.204	1412955	1.276				5.93			106	65	135	
Heptane (NC)	20	0.000	0	0.000				NC				50	150	
Propanenitrile	100	0.020	104091	0.019				-4.76			95	50	150	
Methacrylonitrile	100	0.063	337678	0.061				-3.89			96	50	150	
1,2-Dichloroethane	20	0.291	339242	0.306				5.41			105	65	135	
Isobutyl alcohol	500	0.006	114690	0.004				-33.05			67	50	150	
Methylcyclohexane	50	0.362	1196221	0.432				19.37			119	50	150	

8260 WATER CALCHECK (FORM VII)-- SOP LIMITS

I126908.D	SPCC											
COMPOUND	SPIKE (ug/L)	AVG RF	AC	CCV RF	RF TOL	%DIFFERENCE		CC REC	CCC REC TOL		P/F	
					> OR =	RESULT	TOL (%)	P/F	%	LOW	HIGH	P/F
Trichloroethene	20	0.279	315745	0.285		2.13			102	65	135	
Dibromomethane	20	0.105	111286	0.100		-4.14			96	65	135	
n-Butanol	1000	0.004	135497	0.002		-40.45			60	10	200	
1,2-Dichloropropane (CCC)	20	0.282	330064	0.298		5.77	20		106			
Bromodichloromethane	20	0.323	355164	0.321		-0.79			99	65	135	
1,4-Dioxane	500	0.001	29713	0.001		-14.67			85	10	200	
Methyl methacrylate	20	0.117	103538	0.093		-20.04			80	50	150	
1-Bromo-2-chloroethane	20	0.298	319145	0.288		-3.20			97	65	135	
cis-1,3-Dichloropropene	20	0.398	469591	0.424		6.47			106	65	135	
2-Chloroethyl vinyl ether	20	0.084	91065	0.082		-2.00			98	10	200	
Chlorobenzene-d5 (IS)	16.7	1.000	216076	1.000					100			
Toluene (CCC)	20	5.638	1402109	5.418		-3.89	20		96			
Epichlorohydrin	100	0.057	62086	0.048		-16.50			84	50	150	
2-Nitropropane	20	0.142	33800	0.131		-7.75			92	10	200	
Tetrachloroethene	20	0.933	221453	0.856		-8.28			92	65	135	
4-Methyl-2-pentanone (MIBK)	20	0.569	144597	0.559		-1.72			98	50	150	
trans-1,3-Dichloropropene	20	1.452	348409	1.346		-7.30			93	65	135	
1,1,2-Trichloroethane	20	0.769	166145	0.642		-16.47			84	65	135	
4-Methyl-2-pentanone (MIBC)	100	0.135	83984	0.065		-51.76			48	50	150	Q
Ethyl methacrylate	20	1.081	227803	0.880		-18.53			81	50	150	
Dibromochloromethane	20	0.829	193779	0.749		-9.67			90	65	135	
1,3-Dichloropropane	20	1.562	352024	1.360		-12.88			87	65	135	
1,2-Dibromoethane (EDB)	20	0.680	150105	0.580		-14.64			85	65	135	
2-Hexanone	20	0.349	83332	0.322		-7.84			92	50	150	
Chlorobenzene (SPCC)	20	3.474	864765	3.342	0.30	-3.81			96	65	135	
1-Chlorohexane	20	1.303	389354	1.505		15.48			115	65	135	
Ethylbenzene (CCC)	20	1.970	507995	1.963		-0.35	20		100			
1,1,1,2-Tetrachloroethane	20	1.063	260871	1.008		-5.20			95	65	135	
m&p-Xylene	40	2.441	1274208	2.462		0.85			101	65	135	
o-Xylene	20	2.262	590640	2.282		0.91			101	65	135	
Bromoform (SPCC)	20	0.371	87666	0.339	0.10	-8.59			91	50	150	
Styrene	20	3.350	918205	3.548		5.91			106	65	135	
Isopropylbenzene	20	5.331	1519721	5.873		10.17			110	65	135	
Bromobenzene	20	1.134	288953	1.117		-1.54			98	65	135	
n-Propylbenzene	20	1.511	390038	1.507		-0.23			100	65	135	
1,1,2,2-Tetrachloroethane (SPCC)	20	0.797	183615	0.710	0.30	-10.97			89	65	135	
1,4-Dichlorobenzene-d4 (IS)	16.7	1.000	300940	1.000					100			
2-Chlorotoluene	20	0.970	341166	0.947		-2.42			98	65	135	
Cyclohexanone	100	0.010	0	0.000		-100.00			0			
1,2,3-Trichloropropane	20	0.200	54611	0.152		-24.30			76	65	135	
trans-1,4-Dichloro-2-butene	20	0.148	54770	0.152		2.52			103	50	150	
3-Ethyltoluene	20	4.129	1484463	4.119		-0.24			100	65	135	
4-Chlorotoluene	20	0.962	338777	0.940		-2.26			98	65	135	
1,3,5-Trimethylbenzene	20	3.487	1204781	3.343		-4.13			96	65	135	
2-Ethyltoluene	20	4.185	1465372	4.066		-2.85			97	65	135	

8260 WATER CALCHECK (FORM VII)-- SOP LIMITS

I126908.D						SPCC							
	SPIKE	AVG RF	AC	CCV RF	RF TOL	%DIFFERENCE	CC REC	CCC REC TOL					
COMPOUND	(ug/L)				> OR =	P/F	RESULT	TOL (%)	P/F	%	LOW	HIGH	P/F
tert-Butylbenzene	20	1.914	685957	1.903			-0.55			99	65	135	
Pentachloroethane	50	0.487	0	0.000			100.00			0	50	150	Q
1,2,4-Trimethylbenzene	20	3.492	1210290	3.358			-3.83			96	65	135	
sec-Butylbenzene	20	4.259	1582697	4.391			3.11			103	65	135	
p-Isopropyltoluene	20	3.640	1288641	3.576			-1.77			98	65	135	
1,3-Dichlorobenzene	20	1.728	586946	1.629			-5.75			94	65	135	
1,4-Dichlorobenzene	20	1.829	597806	1.659			-9.33			91	65	135	
Benzyl chloride	20	0.267	55300	0.153			-42.47			58	10	200	
n-Butylbenzene	20	0.850	300190	0.833			-1.98			98	65	135	
1,2-Dichlorobenzene	20	1.437	475901	1.320			-8.12			92	65	135	
1,3,5-Trichlorobenzene (NC)	50	0.000	0	0.000			NC				65	135	
1,2-Dibromo-3-chloropropane (DBC)	20	0.086	17858	0.050			-42.13			58	50	150	
Hexachlorobutadiene	20	0.436	149069	0.414			-5.14			95	50	150	
1,2,4-Trichlorobenzene	20	0.767	288083	0.799			4.15			104	50	150	
Naphthalene	20	1.116	431962	1.199			7.40			107	50	150	
1,2,3-Trichlorobenzene	20	0.545	194628	0.540			-0.91			99	50	150	
Dibromofluoromethane (Surr)	16.7	0.244	224719	0.243			-0.26			100	84	116	
1,2-Dichloroethane-d4 (Surr)	16.7	0.139	125694	0.136			-2.21			98	73	126	
Toluene-d8 (Surr)	16.7	0.959	973973	1.053			9.82			110	89	119	
1,4-Bromofluorobenzene (Surr)	16.7	1.561	348975	1.615			3.46			103	80	116	

NT

Q - Failed criteria
 NC-Not Calibrated

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY (Form VIII)

30

JAN 27 2009

BFB TIME IF NOT IN CCAL

File ID	Calcheck	Sample Name	FB Area	%	RT	CBD5 Area	%	RT	14DCBD4 Area	%	RT	Date/Time
I126908.D		CCV,REGC	924953		6.297	216076		9.4239	300940		11.006	26 Jan 2009 9:15 am ✓
Upper Limit			1849906	200		432152	200		601880	200		
Lower Limit			462476.5	50		108038	50		150470	50		

Sample	Sample Name	FB Area	%	RT	CBD5 Area	%	RT	14DCBD4 Area	%	RT	Date/Time
I126911.D	BATCH-BLK1@1,REGC	864731	93	6.295	186995	87	9.4222	252378	84	11.004	26 Jan 2009 10:37 am
I126912.D	ASA0148-01 @1X ,REGC	830237	90	6.295	174391	81	9.4223	229035	76	11.004	26 Jan 2009 11:04 am
I126913.D	ASA0086-01 @1X A,REGC	786284	85	6.296	171658	79	9.4227	233481	78	11.004	26 Jan 2009 11:32 am
I126914.D	ASA0086-02 @1X A,REGC	771905	83	6.301	171111	79	9.4215	231332	77	11.003	26 Jan 2009 11:59 am
I126915.D	ASA0086-03 @1X A,REGC	754020	82	6.295	162460	75	9.422	216689	72	11.004	26 Jan 2009 12:26 pm
I126916.D	ASA0122-12 @1X C,53765	737396	80	6.301	162096	75	9.4215	213996	71	11.003	26 Jan 2009 12:53 pm
I126917.D	ASA0156-02 @1X A,BTEX	736388	80	6.295	159562	74	9.4222	209418	70	11.004	26 Jan 2009 1:21 pm
I126918.D	ASA0156-01 @100X A,BTEX	749510	81	6.301	170994	79	9.4217	234304	78	11.003	26 Jan 2009 1:48 pm
I126919.D	ASA0122-13 @1X C,53765	778234	84	6.298	171725	79	9.4254	230934	77	11.007	26 Jan 2009 2:15 pm
I126920.D	ASA0122-14 @1X C,53765	744116	80	6.296	161310	75	9.4225	215743	72	11.004	26 Jan 2009 2:43 pm
I126921.D	ASA0122-15 @1X C,53765	729419	79	6.298	158307	73	9.4247	211805	70	11.006	26 Jan 2009 3:10 pm
I126922.D	ASA0122-16 @1X E,53765	708062	77	6.3	155799	72	9.4212	207498	69	11.003	26 Jan 2009 3:38 pm
I126923.D	ASA0122-17 @1X C,53765	691317	75	6.295	151064	70	9.4219	202614	67	11.004	26 Jan 2009 4:05 pm
I126924.D	ASA0122-18 @1X B,53765	63550	70	6.304	141701	70	9.4304	2176	67	11.006	26 Jan 2009 4:37 pm
I126925.D	ASA0122-19 @1X B,53765	653263	71	6.297	140485	65	9.4241	186693	62	11.006	26 Jan 2009 5:05 pm
I126926.D	ASA0131-07 @1X A,57989	635042	69	6.297	141976	66	9.4242	189971	63	11.006	26 Jan 2009 5:33 pm
I126927.D	ASA0131-08 @1X A,57989	632727	68	6.302	140566	65	9.4224	189443	63	11.004	26 Jan 2009 6:00 pm
I126928.D	ASA0131-09 @1X A,57989	664429	72	6.301	145135	67	9.4218	192541	64	11.003	26 Jan 2009 6:28 pm
I126929.D	ASA0131-10 @1X A,57989	665136	72	6.298	148326	69	9.4251	197222	66	11.007	26 Jan 2009 6:55 pm
I126930.D	ASA0131-11 @1X A,57989	641618	69	6.298	140720	65	9.4247	181333	60	11.006	26 Jan 2009 7:23 pm
I126931.D	ASA0131-12 @1X A,57989	629141	68	6.295	136198	63	9.4221	179078	60	11.004	26 Jan 2009 7:50 pm
I126932.D	ASA0086-01RE1 @2X A,REGC	637190	69	6.298	140199	65	9.4247	185347	62	11.006	26 Jan 2009 8:17 pm ✓
			0 Q			0 Q			0 Q		
			0 Q			0 Q			0 Q		
			0 Q			0 Q			0 Q		
			0 Q			0 Q			0 Q		
			0 Q			0 Q			0 Q		
			0 Q			0 Q			0 Q		
			0 Q			0 Q			0 Q		
			0 Q			0 Q			0 Q		
			0 Q			0 Q			0 Q		

R01x

QC & Sample Data

TestAmerica
 Austin Laboratory
 Lot Numbers / Lab Sample Numbers / Batch Numbers

MSVOA DATA REVIEW CHECK LIST

22 / 132

9A 27008	

Method / Queue
 82603

Instrument ID
 m57

Analysis Date
 1-27-9

ICAL Date
 11-4-8

Review Item	Bench Analyst		1st Review		2nd Review
	YES	NO	YES	NO	
Tuning					
BFB tuning criteria met	/				/
Mass list, RIC, and mass spectrum included	/				/
Correct BFB included with analytical runs	/				/
12 hour (8260) / 24 hour (624) clock requirements met	/				/
Initial Calibration					
Correct ICAL date on checklist	/				/
Correct ICAL referenced in sample header	/				/
Failing ICVs checked against target analyte list	/				/
Continuing Calibration					
RRF and % Difference within acceptance criteria	/				/
Sample Analysis					
Sample holding times met	/				/
Sample name and header information correct	/				/
RRT of identified cmpds. w/i +/-0.06 RRT units of RRT of std.comp.	/				/
Surrogate recoveries within limits	/				/
Quantified against appropriate standard	/				/
Ions present in standard spectra with abundance of >10% of base ion present in sample spectra			✓		/
Runs(s) within linear range			✓		/
Target analyte list match			✓		/
Quality Control Samples					
Method blanks analyzed at required frequency	/		✓		/
Method blanks less than reporting limits	/		✓		/
LCS (LCSD) spike % recoveries and RPDs within limits			✓		/
MS/MSD spike % recoveries within limits				✓	/
MS/MSD/DUPs RPD within limits				✓	/
Other					
Required forms completed (CCV and IS macro forms)	/		✓		/
Correct methodology used	/		✓		/
Transcriptions checked for accuracy	/		✓		/
All nonconformances written				NA	/
All unused analyses noted on the sequence with the reason			✓		/
All calculations checked at minimum frequency					/
Data checked for potential false positive and false negative results			✓		/
Manual integration checked by 2 nd reviewer					/
Units checked			✓		/

Comment on any "NO" response:

over-cal, dilutions

Bench Analyst 1-27-9M

1st Review JS

2nd Review 1-29-09

Date _____

Date JAN 27 2009

Date and 1/30/09

Austin Laboratory

PAGE #: 16

INSTRUMENT GCMS-II

ANALYST / DATE: L-26-9 PM

SHIFT (Circle): 1 2 3

METHOD / TEST: 82603

COMPUTER CLOCK DATE / TIME:

SOP #: AU-MS-004, current revision

DAILY CHECK <u>Y</u>	COLUMN CHANGED <u>N</u>	P&T MAINT. (Describe) <u>N</u>	
M. PUMP OIL <u>N</u>	TURBO OIL <u>N</u>	FILAMENT CHANGE <u>N</u>	OTHER <u>NA</u>

DAILY CHECK includes sufficient carrier and detector gases, correct column flow/pressure, etc. Column and gases changed as needed. Source cleaned as needed. Mechanical pump oil and turbomolecular pump oil changed semiannually (usually on service contract). OTHER is for minor maintenance performed or for reference to Repair Log for major repairs.

MASS SPECTROMETER CONDITIONS:

Tune File: Atune.u Sampling Rate 2^{**} 4
 Elect Mult. 1224 volts Scan Range 35-300 amu
 Tuning Performance: BFB Interface: Open-Split

GC PROGRAM: 781104W

GC Meth. 781104W Init. Hold 2 min 2nd Temp 210 C
 Inj. Temp 150 C Ramp 9 C/min 2nd Hold 4 min
 Carrier Gas: Helium Final Temp. 85 C 3rd Ramp C/min
 Flow/Pressure 1.3 Final Hold 0 min 3rd Temp C
 Initial Temp. 35 C 2nd Ramp 30 C/min 3rd Hold min

GC COLUMN:

Column ID#: MSVOAID 010 Capillary
 Phases/Loadings: RTXVMS i.d. 0.25 mm Length 30 m
 Injection Type (Circle & Describe): Purge & Trap Tekmar Velocity/Solatek
Split 120:1 Splitless

INSTRUMENT SEQUENCE:

Sample Name, Sample Number, Dilution, etc. Autosampler #

1126901	I81104W	BLANK	
1126902	I81104W	BLANK	
1126903	I81104W	CCV, REG <u>626um</u>	
1126904	I81104W	LCS, REG	
1126905	I81104W	LCSD, REG	
1126906	I81104W	ASA0148-01 @1X, Q MS, REGC	
1126907	I81104W	ASA0148-01 @1X M MSD, REGC	
1126908	I81104W	CCV, REG <u>915um</u>	
1126909	I81104W	BLANK	
1126910	I81104W	BLANK	
1126911	I81104W	BLANK, REG	
1126912	I81104W	ASA0148-01 @1X, REGC	
1126913	I81104W	ASA0086-01 @1X A, REGC	
1126914	I81104W	ASA0086-02 @1X A, REGC	
1126915	I81104W	ASA0086-03 @1X A, REGC	
1126916	I81104W	ASA0122-12 @1X C, 53765	
1126917	I81104W	ASA0156-02 @1X A, BTEX	
1126918	I81104W	ASA0156-01 @100X A, BTEX	
1126919	I81104W	ASA0122-13 @1X C, 53765	
1126920	I81104W	ASA0122-14 @1X C, 53765	
1126921	I81104W	ASA0122-15 @1X C, 53765	
1126922	I81104W	ASA0122-16 @1X E, 53765	
1126923	I81104W	ASA0122-17 @1X C, 53765	
1126924	I81104W	ASA0122-18 @1X D, 53765	
1126925	I81104W	ASA0122-19 @1X B, 53765	
1126926	I81104W	ASA0131-07 @1X A, 57989	
1126927	I81104W	ASA0131-08 @1X A, 57989	
1126928	I81104W	ASA0131-09 @1X A, 57989	
1126929	I81104W	ASA0131-10 @1X A, 57989	
1126930	I81104W	ASA0131-11 @1X A, 57989	
1126931	I81104W	ASA0131-12 @1X A, 57989	
1126932	I81104W	ASA0086-01RE @2X A, CIS	

1-27-9 PM

MSD

0617pm

Sequence Name: C:\HPCHEM\1\SEQUENCE\I012609.S

24/132

Comment:

Operator: DY

Data Path: C:\HPCHEM\1\DATA\I012609.B\

Pre-Seq Cmd:

Post-Seq Cmd:

9A27008



Method Sections To Run On A Barcode Mismatch
 (X) Full Method (X) Inject Anyway
 () Reprocessing Only () Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Blank	1	I126901	I81104W	BLANK <i>cleaning blank</i>
2 Blank	2	I126902	I81104W	BLANK <i>blank</i>
3 Blank	3	I126903	I81104W	CCV, REG <i>0626 am</i>
4 Blank	4	I126904	I81104W	LCS, REG
5 Blank	5	I126905	I81104W	LCSD, REG
6 Blank	6	I126906	I81104W	ASA0148-01 @1X Q, MS, REGC
7 Blank	7	I126907	I81104W	ASA0148-01 @1X M, MSD, REGC
8 Blank	8	I126908	I81104W	CCV, REG <i>0915 am</i>
9 Blank	9	I126909	I81104W	BLANK <i>cleaning blank</i>
10 Blank	10	I126910	I81104W	BLANK
11 Blank	11	I126911	I81104W	BLANK, REG
12 Blank	12	I126912	I81104W	ASA0148-01 0@1X, REGC <i>Parax</i>
13 Blank	13	I126913	I81104W	ASA0086-01 @1X A, REGC
14 Blank	14	I126914	I81104W	ASA0086-02 @1X A, REGC
15 Blank	15	I126915	I81104W	ASA0086-03 @1X A, REGC
16 Blank	16	I126916	I81104W	ASA0122-12 @1X C, 53765
17 Blank	17	I126917	I81104W	ASA0156-02 @1X A, BTEX
18 Blank	18	I126918	I81104W	ASA0156-01 @100X A, BTEX
19 Blank	19	I126919	I81104W	ASA0122-13 @1X C, 53765
20 Blank	20	I126920	I81104W	ASA0122-14 @1X C, 53765
21 Blank	21	I126921	I81104W	ASA0122-15 @1X C, 53765
22 Blank	22	I126922	I81104W	ASA0122-16 @1X E, 53765
23 Blank	23	I126923	I81104W	ASA0122-17 @1X C, 53765
24 Blank	24	I126924	I81104W	ASA0122-18 @1X D, 53765 <i>MSD</i>
25 Blank	25	I126925	I81104W	ASA0122-19 @1X B, 53765
26 Blank	26	I126926	I81104W	ASA0131-07 @1X A, 57989
27 Blank	27	I126927	I81104W	ASA0131-08 @1X A, 57989
28 Blank	28	I126928	I81104W	ASA0131-09 @1X A, 57989
29 Blank	29	I126929	I81104W	ASA0131-10 @1X A, 57989
30 Blank	30	I126930	I81104W	ASA0131-11 @1X A, 57989
31 Blank	31	I126931	I81104W	ASA0131-12 @1X A, 57989
32 Blank	32	I126932	I81104W	ASA0086-01REJ @2X A, CIS <i>0817 pm</i>

156-RUSH

BFB

Data File : C:\HPCHEM\1\DATA\I012609.B\I126903.D Vial: 3
 Acq On : 26 Jan 2009 6:26 am Operator: DY
 Sample : CCV,REG Inst : MSI
 Misc : 9010191 5uL/50mL Multiplr: 1.00
 MS Integration Params: VOA.P
 Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water

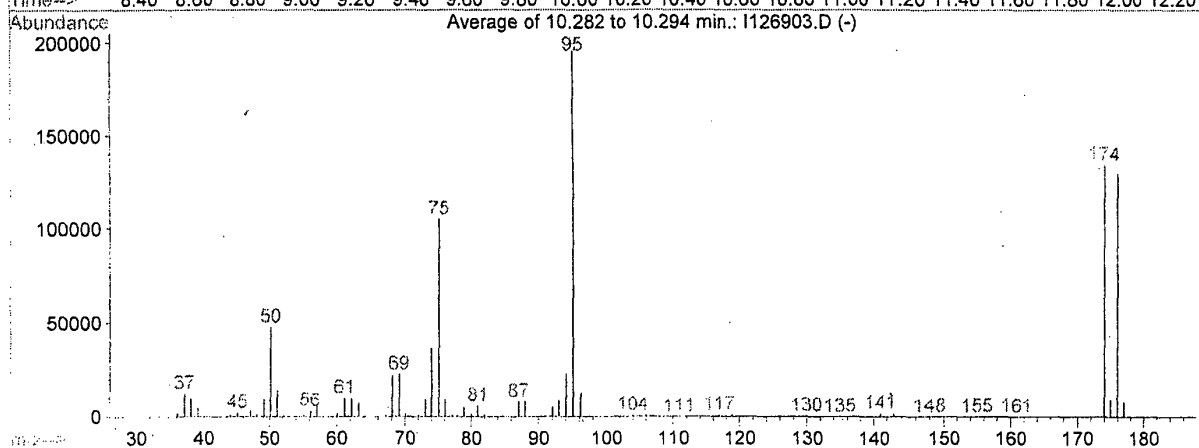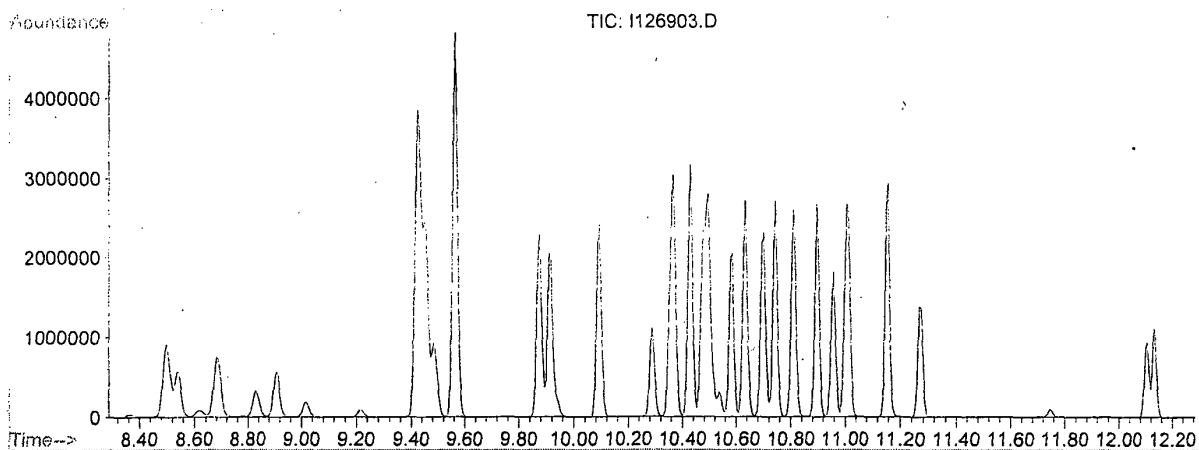

AutoFind: Scans 1511, 1512, 1513; Background Corrected with Scan 1505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	47832	PASS
75	95	30	60	53.8	105237	PASS
95	95	100	100	100.0	195627	PASS
96	95	5	9	6.8	13301	PASS
173	174	0.00	2	0.4	591	PASS
174	95	50	100	68.8	134555	PASS
175	174	5	9	7.1	9592	PASS
176	174	95	101	96.6	130029	PASS
177	176	5	9	6.5	8430	PASS

WMT
1/30/09

Directory: h:\msi\i012609.b

Injection Log

JB JAN 27 2009 26 / 132

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	1	i126901.d	1.	BLANK	1,1, 9010001 5uL/50mL	26 Jan 09 05:31
2	2	i126902.d	1.	BLANK	1,1, 9010225 5uL/50mL	26 Jan 09 05:59
3	3	i126903.d	1.	CCV,REGC	9010191 5uL/50mL	26 Jan 09 06:26
4	4	i126904.d	1.	BATCH-BS1@1,REGC	9010191 5uL/50mL	26 Jan 09 06:53
5	5	i126905.d	1.	BATCH-BSD1@1,REGC	9010191 5uL/50mL	26 Jan 09 07:20
6	6	i126906.d	1.	BATCH-MS1@1X MS,REGC	9010191 4.2uL/42mL; VIALS 1-J,M,Q;G	26 Jan 09 08:21
7	7	i126907.d	1.	BATCH-MSD1@1X MSD,REGC	9010191 4.2uL/42mL; VIALS 1-J,M,Q;G	26 Jan 09 08:48
8	8	i126908.d	1.	CCV,REG	9010191 5uL/50mL	26 Jan 09 09:15
9	9	i126909.d	1.	BLANK	1,1, 9010225 5uL/50mL	26 Jan 09 09:43
10	10	i126910.d	1.	BLANK	1,1, 9010225 5uL/50mL	26 Jan 09 10:10
11	11	i126911.d	1.	BATCH-BLK1@1,REGC	1,1, 9010225 5uL/50mL	26 Jan 09 10:37
12	12	i126912.d	1.	ASA0148-01 @1X ,REGC	VIALS 1-J,M,Q;G	26 Jan 09 11:04
13	13	i126913.d	1.	ASA0086-01 @1X A,REGC		26 Jan 09 11:32
14	14	i126914.d	1.	ASA0086-02 @1X A,REGC		26 Jan 09 11:59
15	15	i126915.d	1.	ASA0086-03 @1X A,REGC		26 Jan 09 12:26
16	16	i126916.d	1.	ASA0122-12 @1X C,53765		26 Jan 09 12:53
17	17	i126917.d	1.	ASA0156-02 @1X A,BTEX		26 Jan 09 13:21
18	18	i126918.d	1.	ASA0156-01 @100X A,BTEX		26 Jan 09 13:48
19	19	i126919.d	1.	ASA0122-13 @1X C,53765		26 Jan 09 14:15
20	20	i126920.d	1.	ASA0122-14 @1X C,53765		26 Jan 09 14:43
21	21	i126921.d	1.	ASA0122-15 @1X C,53765		26 Jan 09 15:10
22	22	i126922.d	1.	ASA0122-16 @1X E,53765		26 Jan 09 15:38
23	23	i126923.d	1.	ASA0122-17 @1X C,53765		26 Jan 09 16:05
24	24	i126924.d	1.	ASA0122-18 @1X D,53765		26 Jan 09 16:37
25	25	i126925.d	1.	ASA0122-19 @1X B,53765		26 Jan 09 17:05
26	26	i126926.d	1.	ASA0131-07 @1X A,57989		26 Jan 09 17:33
27	27	i126927.d	1.	ASA0131-08 @1X A,57989		26 Jan 09 18:00
28	28	i126928.d	1.	ASA0131-09 @1X A,57989		26 Jan 09 18:28
29	29	i126929.d	1.	ASA0131-10 @1X A,57989		26 Jan 09 18:55
30	30	i126930.d	1.	ASA0131-11 @1X A,57989		26 Jan 09 19:23
31	31	i126931.d	1.	ASA0131-12 @1X A,57989		26 Jan 09 19:50
32	32	i126932.d	1.	ASA0086-01RE1 @2X A,CIS	CIS-D	26 Jan 09 20:17

1-29 *msy* 27/132

Data File : H:\MSI.I\I012609.B\I126903.D
 Acq On : 26 Jan 2009 6:26 am
 Sample : CCV,REGC
 Misc : 9010191 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:04 19109

Vial: 3
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

LB JAN 27 2009

**Only worked up:
 Target Analytes**

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	735048	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	173796	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.01	152	244344	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	179787	16.7696	PPB	0.00
Spiked Amount	16.700		Recovery	=	100.42%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	103893	16.9850	PPB	0.00
Spiked Amount	16.700		Recovery	=	101.68%	
64) Toluene-d8 (Surr)	8.08	98	797148	18.8884	PPB	0.00
Spiked Amount	16.700		Recovery	=	113.11%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	285176	17.5542	PPB	0.00
Spiked Amount	16.700		Recovery	=	105.09%	
Target Compounds						
2) Dichlorodifluoromethane	1.59	85	342764	21.1011	PPB	S 98
3) Chloromethane (SPCC)	1.77	50	314569	19.7497	PPB	S 99
4) Vinyl chloride (CCC)	1.86	62	387036	22.4761	PPB	S 99
5) Bromomethane	2.19	94	191262	21.2993	PPB	S 99
6) Ethylene oxide	2.28	44	319165	243.3740	PPB	99
7) Chloroethane	2.32	64	260439	22.3888	PPB	96
8) Trichlorofluoromethane	2.47	101	421060	23.5946	PPB	98
9) Ethyl ether	2.79	59	164036	17.9507	PPB	90
11) 1,1-Dichloroethene (CCC)	2.99	96	218354	19.8077	PPB	85
12) Carbon disulfide	3.01	76	850581	21.9361	PPB	93
13) 1,1,2-Trichlorotrifluoroet	3.04	101	241798	22.7475	PPB	94
14) Propylene oxide	3.12	58	108710	83.5614	PPB	87
15) Iodomethane	3.13	142	286430	17.6771	PPB	89
16) Bromoethane	3.25	108	172766	19.3066	PPB	99
17) Acrolein	3.33	56	73560	116.4827	PPB	98
18) 3-Chloropropene	3.47	41	548080	24.5268	PPB	89
19) Methylene chloride	3.58	84	225172	17.8812	PPB	84
20) Acetone	3.64	58	8191	15.0643	PPB	# 82
21) trans-1,2-Dichloroethene	3.75	96	252376	20.4035	PPB	89
22) Methyl acetate	3.77	74	39984	42.4022	PPB	# 63
23) Hexane	3.83	86	94487	22.9067	PPB	# 63
24) Methyl tert-butyl ether (M)	3.86	73	435267	16.9375	PPB	# 69
25) tert-Butyl alcohol	3.98	59	148349	297.0840	PPB	81
26) Acetonitrile	4.11	40	37755	84.9625	PPB	89
27) Isopropyl ether	4.25	45	1000289	22.0176	PPB	93
28) 2-Chloro-1,3-butadiene	4.36	88	210291	22.0593	PPB	# 68
29) 1,1-Dichloroethane (SPCC)	4.38	63	528534	21.8084	PPB	99
30) Acrylonitrile	4.43	53	202976	87.8386	PPB	98
31) Vinyl acetate	4.65	43	314631	21.4621	PPB	93
32) cis-1,2-Dichloroethene	4.94	96	248121	19.0327	PPB	89
33) 2,2-Dichloropropane	5.04	77	379875	20.9027	PPB	79
34) Cyclohexane	5.14	56	582817	25.8224	PPB	87
35) Bromochloromethane	5.15	130	106434	17.4319	PPB	# 75
37) Chloroform (CCC)	5.24	83	408618	19.5265	PPB	96
38) Carbon tetrachloride	5.36	117	325905	23.0232	PPB	100
41) Tetrahydrofuran	5.40	72	15291	18.0657	PPB	# 77
43) 1,1,1-Trichloroethane	5.43	97	381066	21.7752	PPB	94
44) 1,1-Dichloropropene	5.57	75	392776	23.3495	PPB	81
45) 2-Butanone (MEK)	5.56	43	44822	16.8450	PPB	99
46) Benzene	5.84	78	1127348	21.2700	PPB	95

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 I126903.D I81104W.M Tue Jan 27 13:48:37 2009 RPT1

Data File : H:\MSI.I\I012609.B\I126903.D
 Acq On : 26 Jan 2009 6:26 am
 Sample : CCV,REGC
 Misc : 9010191 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:04 19109

Vial: 3
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
48) Propanenitrile	5.87	54	76498	88.0787	PPB	99
49) Methacrylonitrile	5.89	67	253591	90.8283	PPB #	74
51) 1,2-Dichloroethane	6.06	62	280129	21.9065	PPB	98
52) Isobutyl alcohol	6.13	43	71610	282.8969	PPB	91
53) Methylcyclohexane	6.47	83	979301	61.4867	PPB	90
54) Trichloroethene	6.49	130	248108	20.1977	PPB	94
55) Dibromomethane	6.96	93	87423	18.9527	PPB	91
56) n-Butanol	6.92	56	75775	479.2275	PPB #	78
57) 1,2-Dichloropropane (CCC)	7.08	63	265264	21.3926	PPB	89
58) Bromodichloromethane	7.17	83	291297	20.4786	PPB	97
59) 1,4-Dioxane	7.40	88	17214	311.0425	PPB	98
60) Methyl methacrylate	7.37	69	73145	14.9755	PPB #	70
61) 1-Bromo-2-chloroethane	7.71	63	252379	19.2657	PPB	98
62) cis-1,3-Dichloropropene	7.89	75	368092	21.0045	PPB	84
63) 2-Chloroethyl vinyl ether	7.84	63	67143	18.1856	PPB	90
66) Toluene (CCC)	8.13	91	1141941	19.4631	PPB	97
67) Epichlorohydrin	8.16	57	46452	77.6753	PPB	86
68) 2-Nitropropane	8.36	43	24327	16.5093	PPB	84
69) Tetrachloroethene	8.50	164	171622	17.6752	PPB	95
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	108058	18.2633	PPB	92
71) trans-1,3-Dichloropropene	8.54	75	279003	18.4585	PPB	84
72) 1,1,2-Trichloroethane	8.68	97	132309	16.5398	PPB	95
73) 4-Methyl-2-pentanol (MIBC)	8.62	45	56670	49.2628	PPB	81
74) Ethyl methacrylate	8.69	69	172381	15.7018	PPB	76
75) Dibromochloromethane	8.83	129	150933	17.4938	PPB	99
76) 1,3-Dichloropropane	8.91	76	281224	17.3055	PPB	83
77) 1,2-Dibromoethane (EDB)	9.02	107	116646	16.4936	PPB	100
78) 2-Hexanone	9.22	43	58796	16.1681	PPB	91
79) Chlorobenzene (SPCC)	9.44	112	707342	19.5635	PPB	93
80) 1-Chlorohexane	9.42	55	341612	25.8048	PPB	91
81) Ethylbenzene (CCC)	9.45	106	412996	20.1448	PPB	91
82) 1,1,1,2-Tetrachloroethane	9.49	131	209565	18.9370	PPB	98
83) m&p-Xylene	9.56	106	1053312	41.4608	PPB	93
84) o-Xylene	9.87	106	483716	20.5492	PPB	94
85) Bromoform (SPCC)	9.94	173	70531	18.2865	PPB	99
86) Styrene	9.91	104	752607	21.5857	PPB	95
87) Isopropylbenzene	10.09	105	1257770	22.6729	PPB	97
88) Bromobenzene	10.36	156	231316	19.5994	PPB #	83
89) n-Propylbenzene	10.37	120	318423	20.2533	PPB #	82
90) 1,1,2,2-Tetrachloroethane	10.43	83	153311	18.4843	PPB	99
93) 2-Chlorotoluene	10.48	126	287170	20.2331	PPB	87
95) 1,2,3-Trichloropropane	10.51	110	45226	15.4424	PPB	99
96) trans-1,4-Dichloro-2-buten	10.54	53	46665	21.5163	PPB	78
97) 3-Ethyltoluene	10.43	105	1257078	20.8091	PPB	97
98) 4-Chlorotoluene	10.59	126	281280	19.9895	PPB	87
99) 1,3,5-Trimethylbenzene	10.50	105	1029437	20.1784	PPB	69
100) 2-Ethyltoluene	10.64	105	1242385	20.2893	PPB	75
101) tert-Butylbenzene	10.70	91	589290	21.0452	PPB	87
103) 1,2,4-Trimethylbenzene	10.74	105	1032432	20.2089	PPB	96
104) sec-Butylbenzene	10.81	105	1357879	21.7899	PPB	97
105) p-Isopropyltoluene	10.90	119	1087220	20.4140	PPB	96
106) 1,3-Dichlorobenzene	10.96	146	486992	19.2622	PPB	98
107) 1,4-Dichlorobenzene	11.01	146	498042	18.6079	PPB	98
108) Benzyl chloride	11.16	126	42836	14.1066	PPB #	22
109) n-Butylbenzene	11.16	134	248596	19.9953	PPB #	81

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 I126903.D I81104W.M Tue Jan 27 13:48:37 2009 RPT1

Data File : H:\MSI.I\I012609.B\I126903.D Vial: 3
 Acq On : 26 Jan 2009 6:26 am Operator: DY
 Sample : CCV,REGC Inst : MSI
 Misc : 9010191 5uL/50mL Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:04 19109 Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
110) 1,2-Dichlorobenzene	11.27	146	391594	18.6231	PPB	98
112) 1,2-Dibromo-3-chloropropan	11.75	157	13474	12.1272	PPB	87
113) Hexachlorobutadiene	12.11	225	117805	18.4652	PPB	99
114) 1,2,4-Trichlorobenzene	12.14	180	223244	19.8808	PPB	99
115) Naphthalene	12.33	128	316662	19.3931	PPB	100
116) 1,2,3-Trichlorobenzene	12.43	180	145859	18.2922	PPB	99


Quantitation Report

Data File : H:\MSI.I\I012609.B\I126903.D
 Acq On : 26 Jan 2009 6:26 am
 Sample : CCV,REGC
 Misc : 9010191 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:04 19109

Vial: 3
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration

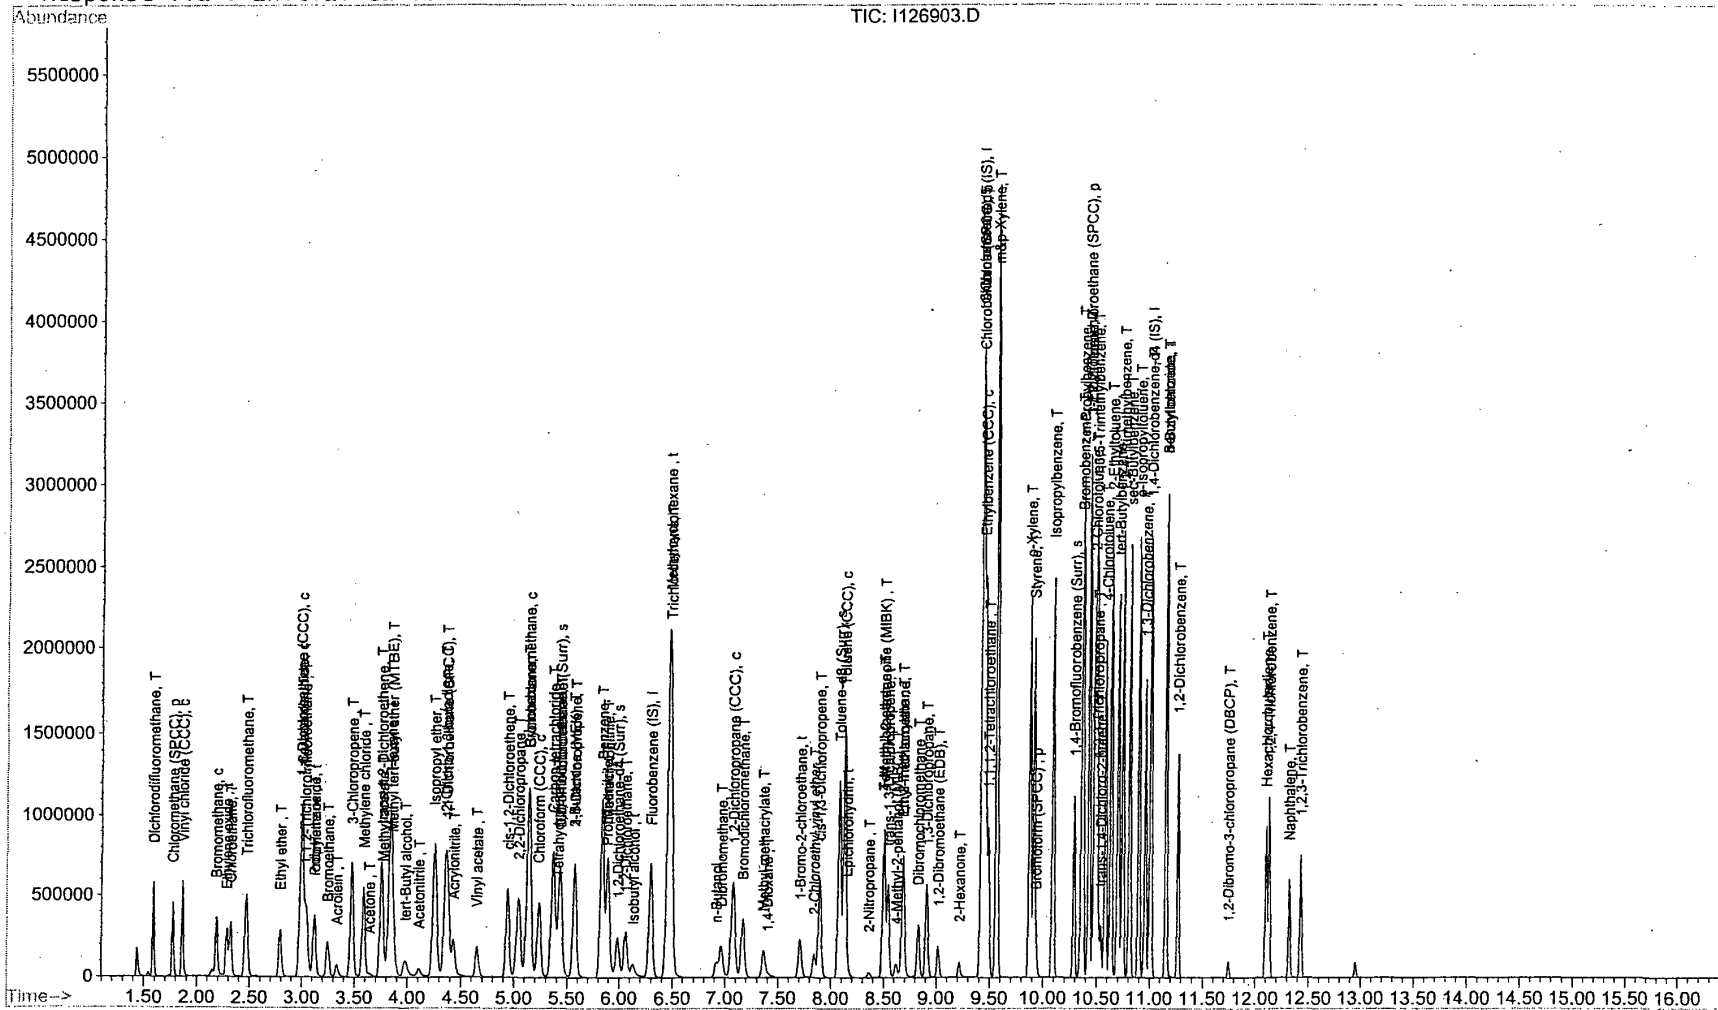

1125-9M31/132

Data File : H:\MSI.I\I012609.B\I126904.D
 Acq On : 26 Jan 2009 6:53 am
 Sample : BATCH-BS1@1,REGC
 Misc : 9010191 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:12 19109

Vial: 4
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

**Only worked up:
 Target Analytes**

JS
 JAN 27 2009

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.29	96	813822	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	188251	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.00	152	259159	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.42	113	199233	16.7846	PPB	0.00
Spiked Amount	16.700		Recovery	=	100.48%	
50) 1,2-Dichloroethane-d4 (Sur)	5.98	67	112288	16.5805	PPB	0.00
Spiked Amount	16.700		Recovery	=	99.28%	
64) Toluene-d8 (Surr)	8.08	98	872820	18.6795	PPB	0.00
Spiked Amount	16.700		Recovery	=	111.86%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	304043	17.2785	PPB	0.00
Spiked Amount	16.700		Recovery	=	103.47%	
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	1.59	85	371866	20.6768	PPB	S 98
3) Chloromethane (SPCC)	1.77	50	369754	20.9673	PPB	S 100
4) Vinyl chloride (CCC)	1.86	62	441893	23.1778	PPB	S 99
5) Bromomethane	2.19	94	223660	22.4964	PPB	S 99
6) Ethylene oxide	2.29	44	339851	234.0636	PPB	98
7) Chloroethane	2.32	64	287816	22.3474	PPB	96
8) Trichlorofluoromethane	2.47	101	459189	23.2406	PPB	99
9) Ethyl ether	2.79	59	190018	18.7812	PPB	91
11) 1,1-Dichloroethene (CCC)	2.99	96	248428	20.3544	PPB	86
12) Carbon disulfide	3.00	76	963169	22.4354	PPB	94
13) 1,1,2-Trichlorotrifluoroet	3.04	101	269438	22.8942	PPB	95
14) Propylene oxide	3.12	58	123958	86.0591	PPB	87
15) Iodomethane	3.13	142	344279	19.0986	PPB	91
16) Bromoethane	3.25	108	196584	19.8419	PPB	99
17) Acrolein	3.33	56	83453	119.3570	PPB	97
18) 3-Chloropropene	3.47	41	620462	25.0783	PPB	90
19) Methylene chloride	3.59	84	254815	18.2765	PPB	86
20) Acetone	3.64	58	9657	16.0413	PPB	88
21) trans-1,2-Dichloroethene	3.75	96	290413	21.2060	PPB	91
22) Methyl acetate	3.77	74	46253	44.3025	PPB	# 61
23) Hexane	3.84	86	105329	23.0634	PPB	# 66
24) Methyl tert-butyl ether (M	3.86	73	499863	17.5684	PPB	# 75
25) tert-Butyl alcohol	3.98	59	161968	292.9612	PPB	83
26) Acetonitrile	4.10	40	40639	82.6004	PPB	86
27) Isopropyl ether	4.26	45	1131416	22.4933	PPB	94
28) 2-Chloro-1,3-butadiene	4.35	88	239789	22.7188	PPB	# 72
29) 1,1-Dichloroethane (SPCC)	4.38	63	589852	21.9827	PPB	99
30) Acrylonitrile	4.43	53	227937	89.0927	PPB	96
31) Vinyl acetate	4.65	43	363187	22.3762	PPB	94
32) cis-1,2-Dichloroethene	4.94	96	283540	19.6443	PPB	91
33) 2,2-Dichloropropane	5.04	77	428460	21.2941	PPB	83
34) Cyclohexane	5.14	56	637516	25.5118	PPB	88
35) Bromochloromethane	5.15	130	120062	17.7605	PPB	# 78
37) Chloroform (CCC)	5.24	83	463613	20.0101	PPB	96
38) Carbon tetrachloride	5.36	117	363867	23.2168	PPB	99
41) Tetrahydrofuran	5.40	72	17095	18.2421	PPB	# 80
43) 1,1,1-Trichloroethane	5.44	97	422239	21.7925	PPB	96
44) 1,1-Dichloropropene	5.57	75	437408	23.4858	PPB	83
45) 2-Butanone (MEK)	5.56	43	53003	17.9915	PPB	96
46) Benzene	5.83	78	1272010	21.6763	PPB	96

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 I126904.D I81104W.M Tue Jan 27 13:49:00 2009 RPT1

Data File : H:\MSI.I\I012609.B\I126904.D
 Acq On : 26 Jan 2009 6:53 am
 Sample : BATCH-BS1@1,REGC
 Misc : 9010191 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:12 19109

Vial: 4
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
48) Propanenitrile	5.88	54	84252	87.6168	PPB	100
49) Methacrylonitrile	5.89	67	283947	91.8567	PPB #	76
51) 1,2-Dichloroethane	6.06	62	304295	21.4930	PPB	99
52) Isobutyl alcohol	6.13	43	77662	277.5153	PPB	95
53) Methylcyclohexane	6.47	83	1081611	61.3370	PPB	91
54) Trichloroethene	6.49	130	279133	20.5238	PPB	95
55) Dibromomethane	6.96	93	96338	18.8638	PPB	91
56) n-Butanol	6.92	56	79579	457.6670	PPB	81
57) 1,2-Dichloropropane (CCC)	7.07	63	295468	21.5219	PPB	90
58) Bromodichloromethane	7.17	83	318187	20.2038	PPB	97
59) 1,4-Dioxane	7.41	88	18119	295.7048	PPB	97
60) Methyl methacrylate	7.37	69	83825	15.4743	PPB	75
61) 1-Bromo-2-chloroethane	7.71	63	278597	19.2085	PPB	98
62) cis-1,3-Dichloropropene	7.89	75	411471	21.2071	PPB	85
63) 2-Chloroethyl vinyl ether	7.84	63	74456	18.2143	PPB	92
66) Toluene (CCC)	8.13	91	1263907	19.8878	PPB	97
67) Epichlorohydrin	8.16	57	51180	79.0099	PPB	90
68) 2-Nitropropane	8.36	43	27343	17.1312	PPB	88
69) Tetrachloroethene	8.50	164	191840	18.2404	PPB	97
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	117748	18.3729	PPB	94
71) trans-1,3-Dichloropropene	8.54	75	307073	18.7556	PPB	87
72) 1,1,2-Trichloroethane	8.68	97	143407	16.5506	PPB	95
73) 4-Methyl-2-pentanol (MIBC)	8.62	45	61761	49.5117	PPB	84
74) Ethyl methacrylate	8.69	69	191027	16.0556	PPB	80
75) Dibromochloromethane	8.83	129	166375	17.8029	PPB	99
76) 1,3-Dichloropropane	8.91	76	308814	17.5441	PPB	86
77) 1,2-Dibromoethane (EDB)	9.01	107	128930	16.8307	PPB	99
78) 2-Hexanone	9.21	43	67062	17.0251	PPB	92
79) Chlorobenzene (SPCC)	9.43	112	767392	19.5946	PPB	94
80) 1-Chlorohexane	9.42	55	368541	25.6948	PPB	91
81) Ethylbenzene (CCC)	9.45	106	452744	20.3879	PPB	87
82) 1,1,1,2-Tetrachloroethane	9.49	131	229416	19.1390	PPB	100
83) m&p-xylene	9.56	106	1150420	41.8061	PPB	95
84) o-Xylene	9.88	106	526193	20.6372	PPB	94
85) Bromoform (SPCC)	9.94	173	75496	18.0708	PPB	100
86) Styrene	9.91	104	814037	21.5549	PPB	95
87) Isopropylbenzene	10.09	105	1359944	22.6323	PPB	97
88) Bromobenzene	10.36	156	252088	19.7193	PPB #	85
89) n-Propylbenzene	10.37	120	349036	20.4958	PPB #	85
90) 1,1,2,2-Tetrachloroethane	10.43	83	159130	17.7127	PPB	99
93) 2-Chlorotoluene	10.47	126	301801	20.0484	PPB #	85
95) 1,2,3-Trichloropropane	10.52	110	47528	15.3007	PPB	99
96) trans-1,4-Dichloro-2-buten	10.54	53	48077	20.9001	PPB	80
97) 3-Ethyltoluene	10.43	105	1346960	21.0224	PPB	98
98) 4-Chlorotoluene	10.58	126	298853	20.0243	PPB	89
99) 1,3,5-Trimethylbenzene	10.49	105	1095184	20.2399	PPB	69
100) 2-Ethyltoluene	10.63	105	1326045	20.4176	PPB	75
101) tert-Butylbenzene	10.70	91	625495	21.0612	PPB	89
103) 1,2,4-Trimethylbenzene	10.74	105	1089020	20.0979	PPB	97
104) sec-Butylbenzene	10.81	105	1440481	21.7940	PPB	97
105) p-Isopropyltoluene	10.90	119	1157513	20.4914	PPB	96
106) 1,3-Dichlorobenzene	10.96	146	515758	19.2338	PPB	99
107) 1,4-Dichlorobenzene	11.02	146	525999	18.5290	PPB	99
108) Benzyl chloride	11.16	126	46610	14.3910	PPB #	31
109) n-Butylbenzene	11.16	134	267853	20.3126	PPB #	86

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 I126904.D I81104W.M Tue Jan 27 13:49:00 2009 RPT1

Data File : H:\MSI.I\I012609.B\I126904.D Vial: 4
 Acq On : 26 Jan 2009 6:53 am Operator: DY
 Sample : BATCH-BS1@1,REGC Inst : MSI
 Misc : 9010191 5uL/50mL Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:12 19109 Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
110) 1,2-Dichlorobenzene	11.27	146	418801	18.7784	PPB	98
112) 1,2-Dibromo-3-chloropropan	11.75	157	14735	12.4614	PPB	91
113) Hexachlorobutadiene	12.10	225	129994	19.2110	PPB	100
114) 1,2,4-Trichlorobenzene	12.13	180	243928	20.4810	PPB	100
115) Naphthalene	12.32	128	349566	20.1845	PPB	100
116) 1,2,3-Trichlorobenzene	12.43	180	160054	18.9249	PPB	99


Quantitation Report

Data File : H:\MSI.I\I012609.B\I126904.D
 Acq On : 26 Jan 2009 6:53 am
 Sample : BATCH-BS1@1.REGC
 Misc : 9010191 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:12 19109

Vial: 4
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration

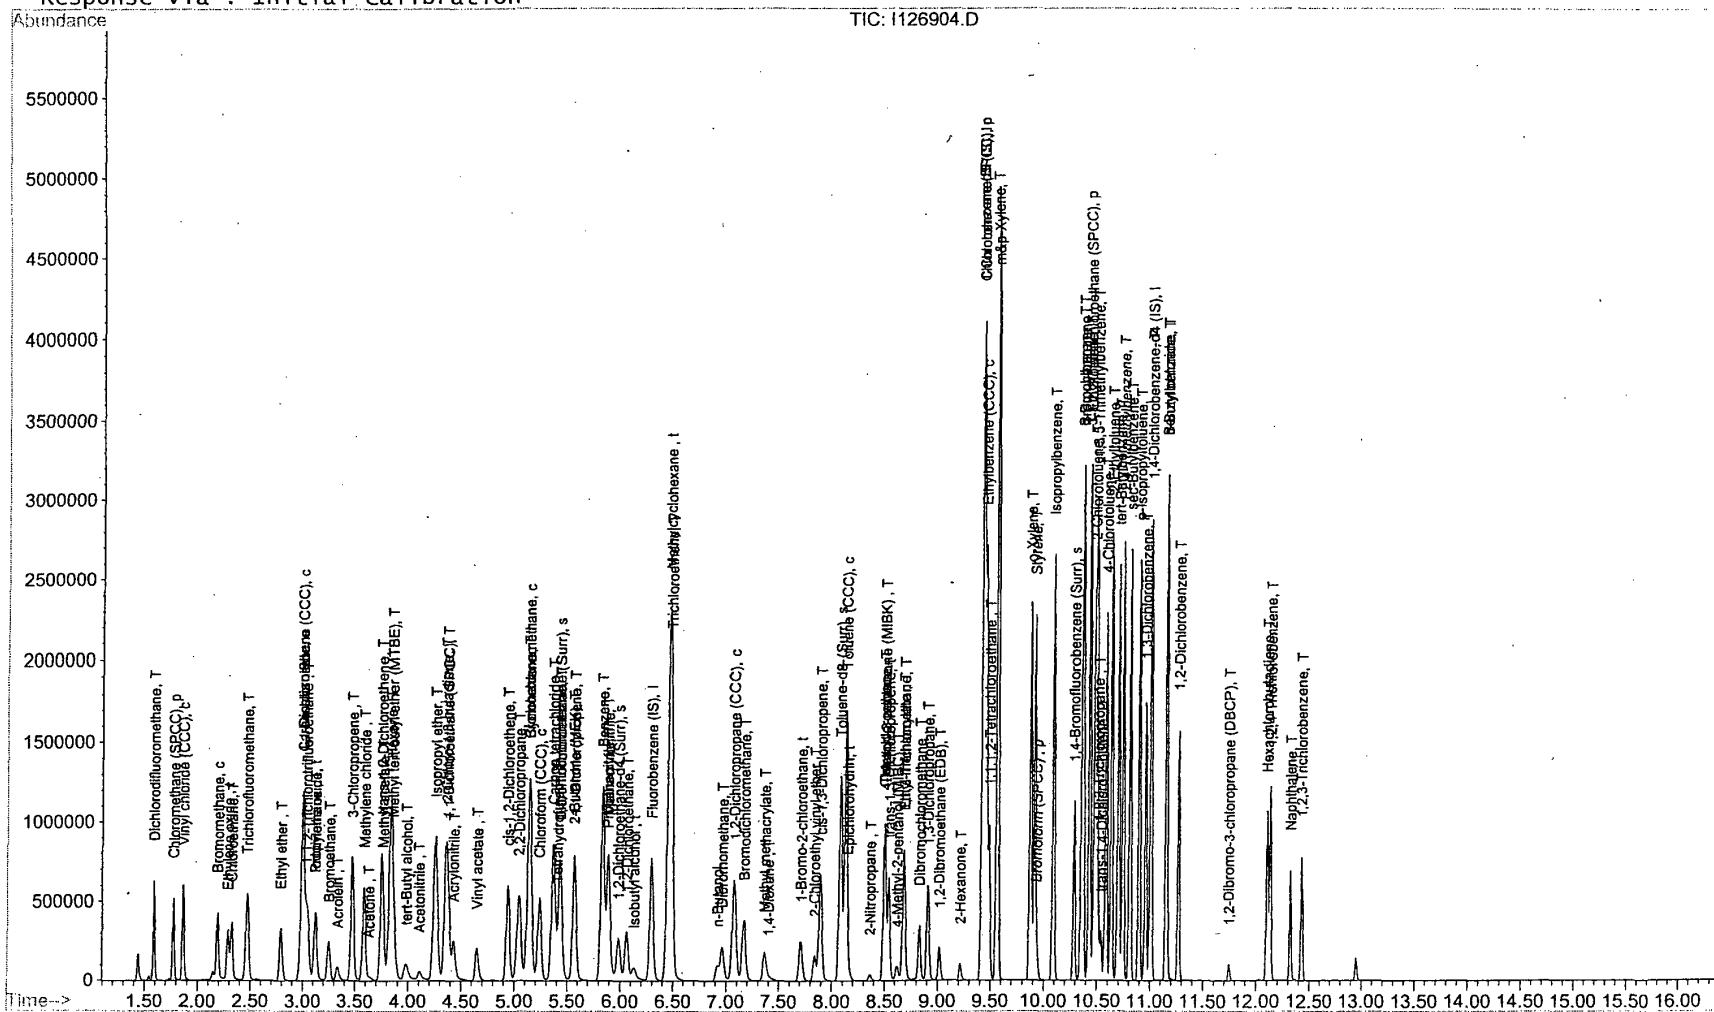

Quantitation Report (QT Reviewed)

1-29-9/11035/132

Data File : H:\MSI.I\I012609.B\I126905.D
 Acq On : 26 Jan 2009 7:20 am
 Sample : BATCH-bsd1@1,REGC
 Misc : 9010191 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:13 19109

Vial: 5
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

JS

JAN 27 2009

Only worked up:
 Target Analytes

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.29	96	863283	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	199370	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.00	152	272774	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	205385	16.3115	PPB	0.00
Spiked Amount	16.700		Recovery	=	97.66%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	112630	15.6782	PPB	0.00
Spiked Amount	16.700		Recovery	=	93.89%	
64) Toluene-d8 (Surr)	8.08	98	900530	18.1684	PPB	0.00
Spiked Amount	16.700		Recovery	=	108.80%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	314442	16.8729	PPB	0.00
Spiked Amount	16.700		Recovery	=	101.02%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.59	85	375928	19.7050	PPB	S 98
3) Chloromethane (SPCC)	1.77	50	394783	21.1040	PPB	S 99
4) Vinyl chloride (CCC)	1.87	62	444553	21.9814	PPB	S 99
5) Bromomethane	2.19	94	234991	22.2818	PPB	S 99
6) Ethylene oxide	2.29	44	343219	222.8398	PPB	99
7) Chloroethane	2.32	64	293321	21.4700	PPB	97
8) Trichlorofluoromethane	2.47	101	464399	22.1576	PPB	99
9) Ethyl ether	2.79	59	192607	17.9464	PPB	92
11) 1,1-Dichloroethene (CCC)	2.99	96	254082	19.6249	PPB	88
12) Carbon disulfide	3.00	76	977925	21.4740	PPB	95
13) 1,1,2-Trichlorotrifluoroet	3.04	101	274883	22.0186	PPB	95
14) Propylene oxide	3.12	58	125622	82.2175	PPB	89
15) Iodomethane	3.12	142	328908	17.3074	PPB	92
16) Bromoethane	3.25	108	200625	19.0896	PPB	100
17) Acrolein	3.34	56	86221	116.2507	PPB	99
18) 3-Chloropropene	3.48	41	619348	23.5990	PPB	91
19) Methylene chloride	3.59	84	260216	17.5945	PPB	88
20) Acetone	3.64	58	9858	15.4370	PPB	85
21) trans-1,2-Dichloroethene	3.75	96	295248	20.3239	PPB	91
22) Methyl acetate	3.77	74	48164	43.4897	PPB	# 70
23) Hexane	3.84	86	108404	22.3768	PPB	# 69
24) Methyl tert-butyl ether (M	3.86	73	515364	17.0754	PPB	78
25) tert-Butyl alcohol	3.98	59	160961	274.4592	PPB	85
26) Acetonitrile	4.11	40	40454	77.5134	PPB	88
27) Isopropyl ether	4.26	45	1145025	21.4596	PPB	94
28) 2-Chloro-1,3-butadiene	4.35	88	242664	21.6740	PPB	# 74
29) 1,1-Dichloroethane (SPCC)	4.38	63	590357	20.7409	PPB	100
30) Acrylonitrile	4.43	53	234523	86.4149	PPB	100
31) Vinyl acetate	4.65	43	369281	21.4482	PPB	94
32) cis-1,2-Dichloroethene	4.94	96	288617	18.8504	PPB	92
33) 2,2-Dichloropropane	5.05	77	432134	20.2462	PPB	84
34) Cyclohexane	5.14	56	649034	24.4847	PPB	89
35) Bromochloromethane	5.14	130	124969	17.4273	PPB	# 81
37) Chloroform (CCC)	5.24	83	465051	18.9222	PPB	97
38) Carbon tetrachloride	5.36	117	362590	21.8098	PPB	100
41) Tetrahydrofuran	5.39	72	16672	16.7714	PPB	# 78
43) 1,1,1-Trichloroethane	5.44	97	427873	20.8180	PPB	95
44) 1,1-Dichloropropene	5.57	75	443972	22.4725	PPB	85
45) 2-Butanone (MEK)	5.56	43	50456	16.1457	PPB	100
46) Benzene	5.84	78	1295493	20.8116	PPB	95

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 I126905.D I81104W.M Tue Jan 27 13:49:25 2009 RPT1

Data File : H:\MSI.I\I012609.B\I126905.D
 Acq On : 26 Jan 2009 7:20 am
 Sample : BATCH-BSD101,REGC
 Misc : 9010191 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:13 19109

Vial: 5
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
48) Propanenitrile	5.87	54	85653	83.9704	PPB	99
49) Methacrylonitrile	5.89	67	287362	87.6353	PPB #	78
51) 1,2-Dichloroethane	6.06	62	306817	20.4295	PPB	98
52) Isobutyl alcohol	6.13	43	75509	256.0223	PPB	95
53) Methylcyclohexane	6.46	83	1105102	59.0785	PPB	92
54) Trichloroethene	6.49	130	285164	19.7659	PPB	95
55) Dibromomethane	6.96	93	96783	17.8652	PPB	92
56) n-Butanol	6.91	56	76532	420.5475	PPB	83
57) 1,2-Dichloropropane (CCC)	7.08	63	298445	20.4933	PPB	91
58) Bromodichloromethane	7.16	83	318898	19.0888	PPB	98
59) 1,4-Dioxane	7.41	88	17559	270.1470	PPB	89
60) Methyl methacrylate	7.37	69	85351	14.8837	PPB	75
61) 1-Bromo-2-chloroethane	7.71	63	281744	18.3125	PPB	98
62) cis-1,3-Dichloropropene	7.89	75	417143	20.2676	PPB	86
63) 2-Chloroethyl vinyl ether	7.84	63	74368	17.1505	PPB	89
66) Toluene (CCC)	8.13	91	1276748	18.9694	PPB	97
67) Epichlorohydrin	8.16	57	52216	76.1136	PPB	92
68) 2-Nitropropane	8.36	43	27928	16.5219	PPB	89
69) Tetrachloroethene	8.50	164	196142	17.6093	PPB	97
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	121380	17.8834	PPB	94
71) trans-1,3-Dichloropropene	8.54	75	307354	17.7258	PPB	86
72) 1,1,2-Trichloroethane	8.68	97	145465	15.8518	PPB	95
73) 4-Methyl-2-pentanol (MIBC)	8.62	45	61538	47.1019	PPB	85
74) Ethyl methacrylate	8.69	69	191894	15.2481	PPB	81
75) Dibromochloromethane	8.83	129	168129	16.9873	PPB	100
76) 1,3-Dichloropropane	8.91	76	313190	16.8004	PPB	86
77) 1,2-Dibromoethane (EDB)	9.02	107	131480	16.2064	PPB	99
78) 2-Hexanone	9.21	43	67386	16.1533	PPB	92
79) Chlorobenzene (SPCC)	9.43	112	778888	18.7790	PPB	94
80) 1-Chlorohexane	9.42	55	371362	24.3715	PPB	91
81) Ethylbenzene (CCC)	9.46	106	462471	19.6644	PPB	88
82) 1,1,1,2-Tetrachloroethane	9.49	131	232292	18.2981	PPB	99
83) m&p-Xylene	9.57	106	1163172	39.9121	PPB	95
84) o-Xylene	9.88	106	530816	19.6575	PPB	95
85) Bromoform (SPCC)	9.94	173	75507	17.0655	PPB	99
86) Styrene	9.91	104	817650	20.4431	PPB	95
87) Isopropylbenzene	10.09	105	1382757	21.7286	PPB	97
88) Bromobenzene	10.36	156	255055	18.8387	PPB #	86
89) n-Propylbenzene	10.37	120	351733	19.5023	PPB #	87
90) 1,1,2,2-Tetrachloroethane	10.43	83	159793	16.7945	PPB	98
93) 2-Chlorotoluene	10.48	126	310221	19.5791	PPB	88
95) 1,2,3-Trichloropropene	10.52	110	47184	14.4318	PPB	99
96) trans-1,4-Dichloro-2-buten	10.54	53	47577	19.6504	PPB	80
97) 3-Ethyltoluene	10.43	105	1357877	20.1349	PPB	98
98) 4-Chlorotoluene	10.58	126	303147	19.2982	PPB	90
99) 1,3,5-Trimethylbenzene	10.50	105	1105197	19.4055	PPB	68
100) 2-Ethyltoluene	10.64	105	1333974	19.5145	PPB	76
101) tert-Butylbenzene	10.70	91	628101	20.0934	PPB	90
103) 1,2,4-Trimethylbenzene	10.75	105	1104420	19.3648	PPB	97
104) sec-Butylbenzene	10.81	105	1464127	21.0461	PPB	97
105) p-Isopropyltoluene	10.90	119	1176445	19.7870	PPB	96
106) 1,3-Dichlorobenzene	10.96	146	518419	18.3681	PPB	99
107) 1,4-Dichlorobenzene	11.02	146	531428	17.7859	PPB	98
108) Benzyl chloride	11.16	126	44708	13.3922	PPB #	21
109) n-Butylbenzene	11.16	134	269714	19.4329	PPB #	86

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 I126905.D I81104W.M Tue Jan 27 13:49:26 2009 RPT1

Data File : H:\MSI.I\I012609.B\I126905.D
 Acq On : 26 Jan 2009 7:20 am
 Sample : BATCH-BSD101,REGC
 Misc : 9010191 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:13 19109

Vial: 5
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
110) 1,2-Dichlorobenzene	11.27	146	419415	17.8673	PPB	99
112) 1,2-Dibromo-3-chloropropan	11.75	157	14705	11.8864	PPB	90
113) Hexachlorobutadiene	12.10	225	134032	18.8190	PPB	99
114) 1,2,4-Trichlorobenzene	12.13	180	248917	19.8567	PPB	100
115) Naphthalene	12.32	128	356869	19.5776	PPB	100
116) 1,2,3-Trichlorobenzene	12.43	180	165480	18.5899	PPB	99


Quantitation Report

Data File : H:\MSI.I\I012609.B\I126905.D
 Acq On : 26 Jan 2009 7:20 am
 Sample : BATCH-bsd101,REGC
 Misc : 9010191 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:13 19109

Vial: 5
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration

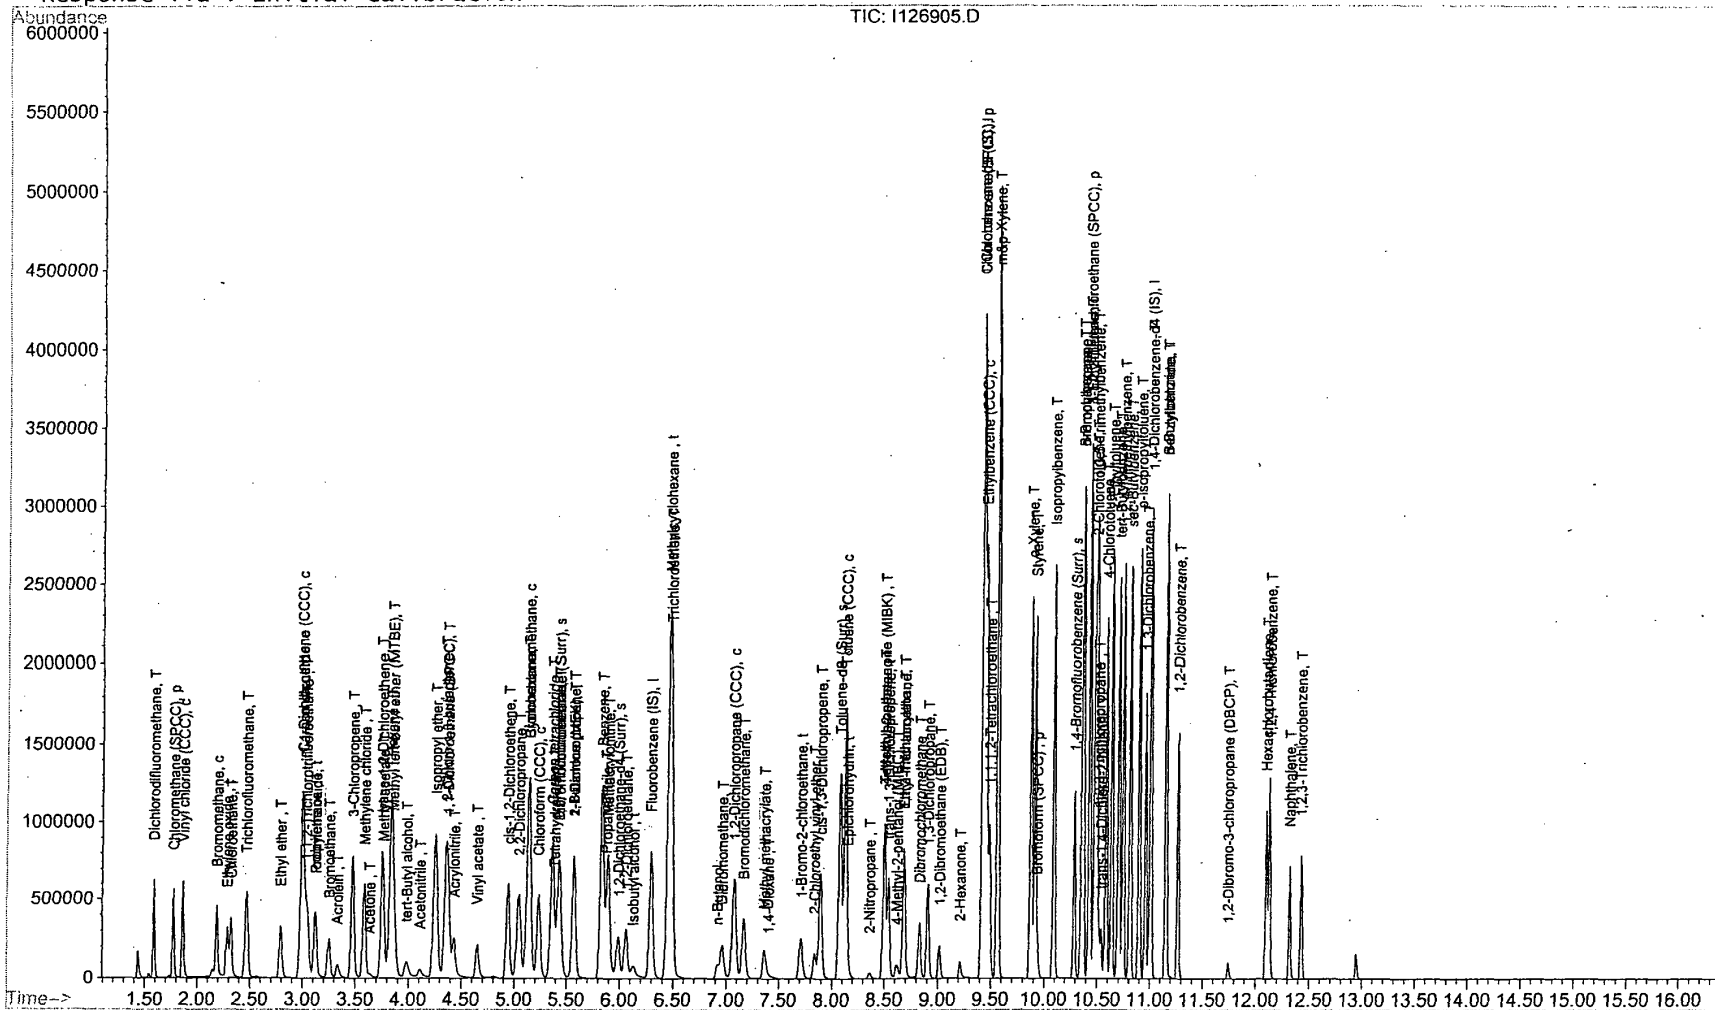

Data File : H:\MSI.I\I012609.B\I126906.D
 Acq On : 26 Jan 2009 8:21 am
 Sample : BATCH-MS1@1X MS,REGC
 Misc : 9010191 4.2uL/42mL; VIALS 1-J,M,Q;G
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:18 19109

Vial: 6
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

1-29-9-23 39/132

Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

JP

Only worked up:
 Target Analytes

JAN 27 2009

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.29	96	896609	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	207524	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.00	152	283186	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	211705	16.1885	PPB	0.00
Spiked Amount	16.700		Recovery	=	96.95%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	113632	15.2297	PPB	0.00
Spiked Amount	16.700		Recovery	=	91.20%	
64) Toluene-d8 (Surr)	8.08	98	932173	18.1077	PPB	0.00
Spiked Amount	16.700		Recovery	=	108.44%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	327516	16.8839	PPB	0.00
Spiked Amount	16.700		Recovery	=	101.08%	
Target Compounds						
2) Dichlorodifluoromethane	1.59	85	432833	21.8445	PPB	S 98
3) Chloromethane (SPCC)	1.77	50	468161	24.0964	PPB	S 99
4) Vinyl chloride (CCC)	1.86	62	512242	24.3869	PPB	S 100
5) Bromomethane	2.19	94	269792	24.6308	PPB	S 100
6) Ethylene oxide	2.29	44	269951	168.7550	PPB	99
7) Chloroethane	2.32	64	324818	22.8917	PPB	97
8) Trichlorofluoromethane	2.47	101	523825	24.0640	PPB	99
9) Ethyl ether	2.79	59	196678	17.6446	PPB	92
11) 1,1-Dichloroethene (CCC)	2.99	96	290058	21.5710	PPB	89
12) Carbon disulfide	3.00	76	1146701	24.2442	PPB	95
13) 1,1,2-Trichlorotrifluoroet	3.04	101	315086	24.3009	PPB	95
14) Propylene oxide	3.12	58	34633	21.8242	PPB	88
15) Iodomethane	3.13	142	362084	18.2805	PPB	92
16) Bromoethane	3.25	108	221593	20.3010	PPB	99
17) Acrolein	3.33	56	87760	113.9276	PPB	100
18) 3-Chloropropene	3.48	41	681626	25.0067	PPB	91
19) Methylene chloride	3.59	84	276554	18.0042	PPB	89
20) Acetone	3.64	58	10339	15.5885	PPB	# 83
21) trans-1,2-Dichloroethene	3.75	96	332856	22.0610	PPB	92
22) Methyl acetate	3.77	74	49129	42.7122	PPB	# 67
23) Hexane	3.84	86	125202	24.8836	PPB	# 74
24) Methyl tert-butyl ether (M)	3.86	73	518414	16.5380	PPB	# 63
25) tert-Butyl alcohol	3.98	59	159761	262.2877	PPB	89
26) Acetonitrile	4.10	40	42164	77.7870	PPB	91
27) Isopropyl ether	4.26	45	1183946	21.3643	PPB	95
28) 2-Chloro-1,3-butadiene	4.35	88	274933	23.6434	PPB	# 75
29) 1,1-Dichloroethane (SPCC)	4.38	63	646122	21.8564	PPB	99
30) Acrylonitrile	4.43	53	234959	83.3577	PPB	97
31) Vinyl acetate	4.65	43	370924	20.7428	PPB	95
32) cis-1,2-Dichloroethene	4.94	96	314950	19.8057	PPB	92
33) 2,2-Dichloropropane	5.05	77	486502	21.9462	PPB	85
34) Cyclohexane	5.14	56	734700	26.6862	PPB	89
35) Bromochloromethane	5.15	130	130150	17.4752	PPB	# 83
37) Chloroform (CCC)	5.24	83	511592	20.0421	PPB	97
38) Carbon tetrachloride	5.36	117	409392	23.7097	PPB	99
41) Tetrahydrofuran	5.40	72	17685	17.1292	PPB	# 87
43) 1,1,1-Trichloroethane	5.44	97	475667	22.2832	PPB	96
44) 1,1-Dichloropropene	5.57	75	499645	24.3505	PPB	86
45) 2-Butanone (MEK)	5.56	43	49890	15.3712	PPB	93
46) Benzene	5.84	78	1406104	21.7490	PPB	96

(#)=qualifier out of range (m)=manual integration (s)=analyte in sublist
 I126906.D I81104W.M Tue Jan 27 13:49:44 2009 RPT1

Data File : H:\MSI.I\I012609.B\I126906.D Vial: 6
 Acq On : 26 Jan 2009 8:21 am Operator: DY
 Sample : BATCH-MS1@1X MS,REGC Inst : MSI
 Misc : 9010191 4.2uL/42mL; VIALS 1-J,M,Q;G Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:18 19109 Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
48) Propanenitrile	5.87	54	85162	80.3858	PPB	98
49) Methacrylonitrile	5.89	67	286138	84.0186	PPB #	78
51) 1,2-Dichloroethane	6.06	62	311093	19.9443	PPB	99
52) Isobutyl alcohol	6.13	43	71324	234.6448	PPB	95
53) Methylcyclohexane	6.47	83	1260942	64.9042	PPB	92
54) Trichloroethene	6.49	130	316792	21.1421	PPB	95
55) Dibromomethane	6.96	93	99773	17.7326	PPB	93
56) n-Butanol	6.92	56	69416	374.8932	PPB	82
57) 1,2-Dichloropropane (CCC)	7.07	63	314934	20.8217	PPB	92
58) Bromodichloromethane	7.17	83	344674	19.8649	PPB	98
59) 1,4-Dioxane	7.40	88	15529	230.0350	PPB	97
60) Methyl methacrylate	7.37	69	84954	14.2954	PPB	77
61) 1-Bromo-2-chloroethane	7.71	63	286740	17.9445	PPB	99
62) cis-1,3-Dichloropropene	7.89	75	430981	20.1617	PPB	87
63) 2-Chloroethyl vinyl ether	7.84	63	1384	0.3073	PPB #	1
66) Toluene (CCC)	8.13	91	1392313	19.8736	PPB	97
67) Epichlorohydrin	8.16	57	48188	67.4822	PPB	78
68) 2-Nitropropane	8.36	43	26822	15.2441	PPB	92
69) Tetrachloroethene	8.50	164	223981	19.3186	PPB	97
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	116756	16.5262	PPB	94
71) trans-1,3-Dichloropropene	8.54	75	313454	17.3673	PPB	87
72) 1,1,2-Trichloroethane	8.68	97	147261	15.4170	PPB	96
73) 4-Methyl-2-pentanol (MIBC)	8.62	45	48833	37.9981	PPB	83
74) Ethyl methacrylate	8.69	69	191146	14.6080	PPB	81
75) Dibromochloromethane	8.83	129	178915	17.3668	PPB	100
76) 1,3-Dichloropropane	8.91	76	313647	16.1638	PPB	87
77) 1,2-Dibromoethane (EDB)	9.02	107	133195	15.7727	PPB	99
78) 2-Hexanone	9.22	43	65329	15.0449	PPB	92
79) Chlorobenzene (SPCC)	9.43	112	838037	19.4112	PPB	94
80) 1-Chlorohexane	9.42	55	409249	25.8950	PPB	91
81) Ethylbenzene (CCC)	9.46	106	501386	20.4814	PPB	88
82) 1,1,1,2-Tetrachloroethane	9.49	131	243625	18.4368	PPB	99
83) m&p-Xylene	9.57	106	1267504	41.7831	PPB	95
84) o-Xylene	9.88	106	579560	20.6193	PPB	95
85) Bromoform (SPCC)	9.94	173	79982	17.3666	PPB	99
86) Styrene	9.91	104	876716	21.0586	PPB	96
87) Isopropylbenzene	10.09	105	1518644	22.9263	PPB	98
88) Bromobenzene	10.36	156	267627	18.9906	PPB #	86
89) n-Propylbenzene	10.37	120	386662	20.5966	PPB #	86
90) 1,1,2,2-Tetrachloroethane	10.43	83	158119	15.9656	PPB	98
93) 2-Chlorotoluene	10.47	126	337370	20.5097	PPB	89
95) 1,2,3-Trichloropropane	10.52	110	46961	13.8354	PPB	99
96) trans-1,4-Dichloro-2-buten	10.54	53	46519	18.5070	PPB	82
97) 3-Ethyltoluene	10.43	105	1487691	21.2488	PPB	98
98) 4-Chlorotoluene	10.58	126	330697	20.2779	PPB	90
99) 1,3,5-Trimethylbenzene	10.50	105	1215330	20.5547	PPB	69
100) 2-Ethyltoluene	10.63	105	1446647	20.3846	PPB	76
101) tert-Butylbenzene	10.70	91	688604	21.2190	PPB	91
103) 1,2,4-Trimethylbenzene	10.74	105	1193126	20.1510	PPB	98
104) sec-Butylbenzene	10.81	105	1642177	22.7375	PPB	97
105) p-Isopropyltoluene	10.90	119	1308991	21.2069	PPB	97
106) 1,3-Dichlorobenzene	10.96	146	559024	19.0785	PPB	99
107) 1,4-Dichlorobenzene	11.02	146	565247	18.2222	PPB	98
108) Benzyl chloride	11.16	126	48335	13.8168	PPB #	16
109) n-Butylbenzene	11.16	134	306108	21.2441	PPB	89

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 I126906.D I81104W.M Tue Jan 27 13:49:45 2009 RPT1

Data File : H:\MSI.I\I012609.B\I126906.D Vial: 6
 Acq On : 26 Jan 2009 8:21 am Operator: DY
 Sample : BATCH-MSI01X MS,REGC Inst : MSI
 Misc : 9010191 4.2uL/42mL; VIALS 1-J,M,Q;G Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:18 19109 Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
110) 1,2-Dichlorobenzene	11.27	146	440004	18.0552	PPB	99
112) 1,2-Dibromo-3-chloropropan	11.75	157	14710	11.5033	PPB	89
113) Hexachlorobutadiene	12.10	225	156588	21.1777	PPB	100
114) 1,2,4-Trichlorobenzene	12.14	180	264141	20.2965	PPB	100
115) Naphthalene	12.32	128	367468	19.4179	PPB	100
116) 1,2,3-Trichlorobenzene	12.43	180	171818	18.5922	PPB	99


Quantitation Report

Data File : H:\MSI.I\I012609.B\I126906.D
Acq On : 26 Jan 2009 8:21 am
Sample : BATCH-MSI@1X MS,REGC
Misc : 9010191 4.2uL/42mL; VIALS 1-J,M,Q;G
MS Integration Params: VOA.P
Quant Time: Jan 27 12:18 19109

Vial: 6
Operator: DY
Inst : MSI
Multiplr: 1.00

Quant Results File: I81104W.RES

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Tue Nov 11 14:35:13 2008
Response via : Initial Calibration

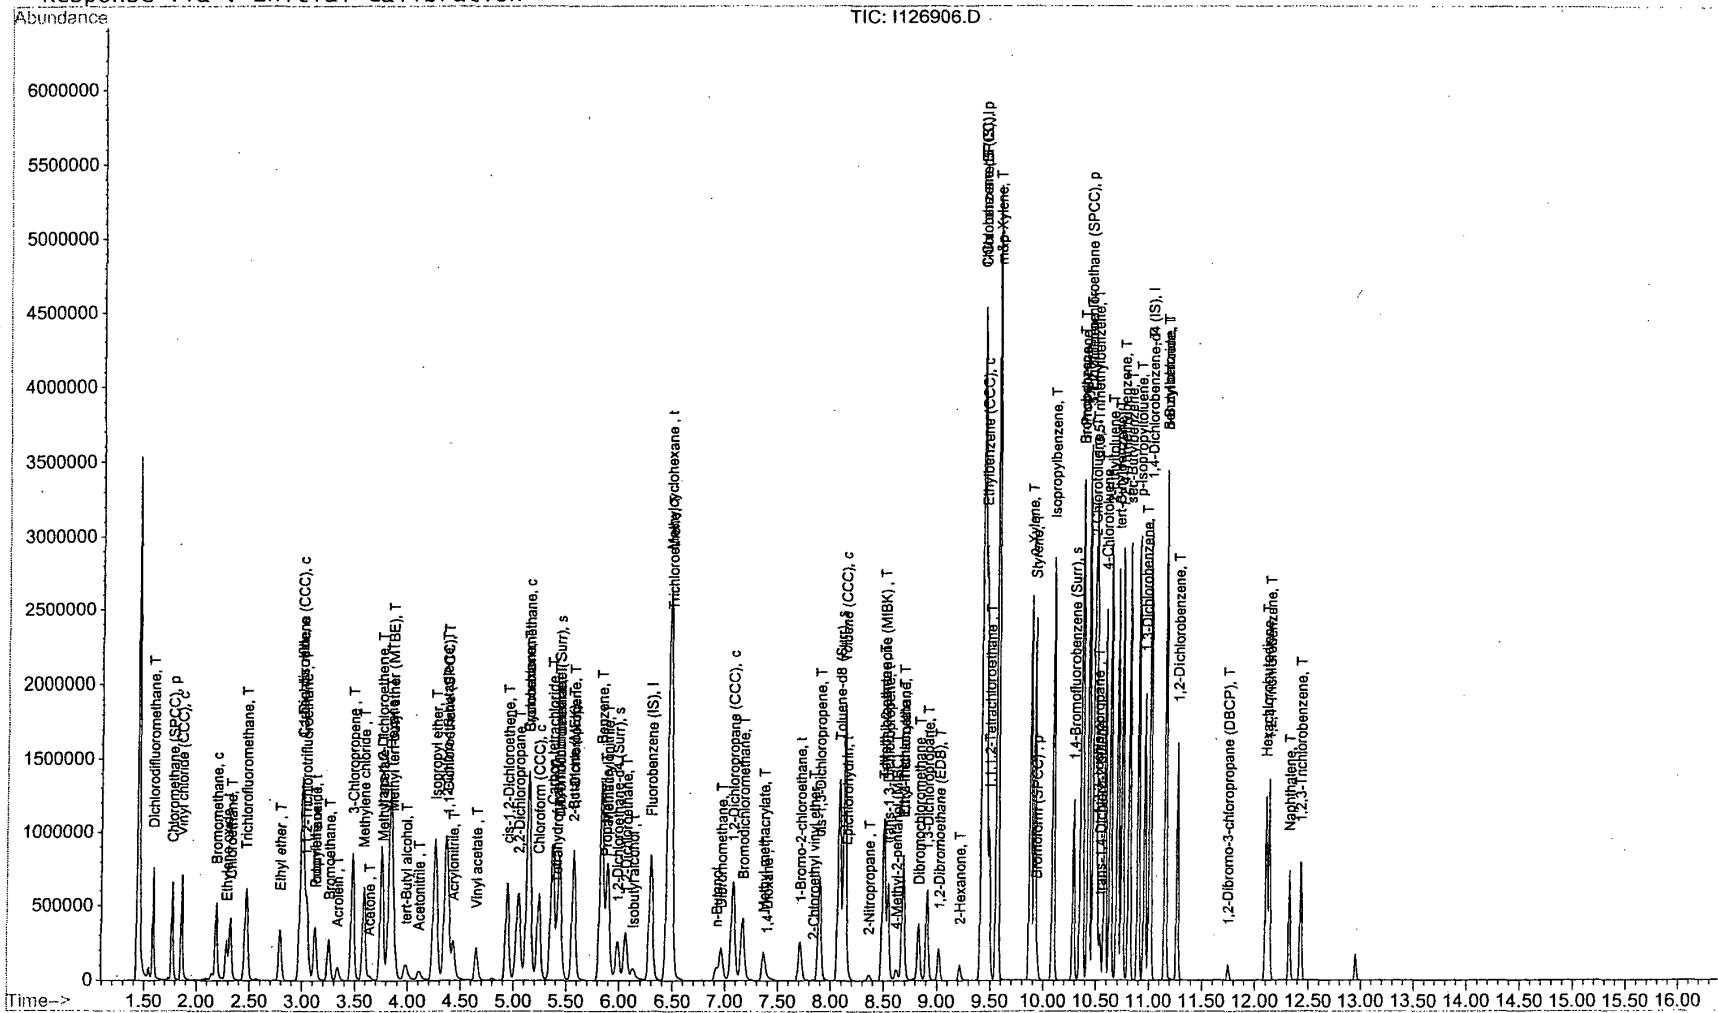

Data File : H:\MSI.I\I012609.B\I126907.D
 Acq On : 26 Jan 2009 8:48 am
 Sample : BATCH-MSD1@1X MSD,REGC
 Misc : 9010191 4.2uL/42mL; VIALS 1-J,M,Q;G
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:48 19109

Vial: 7
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

1-29-9m

Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

53

JAN 27 2009

**Only worked up:
Target Analytes**

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	911243	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.43	119	212928	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.01	152	293390	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	222446	16.7367	PPB	0.00
Spiked Amount	16.700		Recovery	=	100.24%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	123535	16.2911	PPB	0.00
Spiked Amount	16.700		Recovery	=	97.54%	
64) Toluene-d8 (Surr)	8.08	98	961838	18.3839	PPB	0.00
Spiked Amount	16.700		Recovery	=	110.06%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	337797	16.9719	PPB	0.00
Spiked Amount	16.700		Recovery	=	101.62%	
Target Compounds						
2) Dichlorodifluoromethane	1.59	85	449626	22.3276	PPB	S 98
3) Chloromethane (SPCC)	1.77	50	487157	24.6714	PPB	S 99
4) Vinyl chloride (CCC)	1.86	62	525035	24.5946	PPB	S 99
5) Bromomethane	2.19	94	289799	26.0325	PPB	S 99
6) Ethylene oxide	2.28	44	164493	101.1784	PPB	98
7) Chloroethane	2.32	64	339573	23.5473	PPB	97
8) Trichlorofluoromethane	2.47	101	536962	24.2713	PPB	99
9) Ethyl ether	2.79	59	219468	19.3729	PPB	93
11) 1,1-Dichloroethene (CCC)	2.99	96	302769	22.1546	PPB	90
12) Carbon disulfide	3.01	76	1149497	23.9130	PPB	95
13) 1,1,2-Trichlorotrifluoroet	3.04	101	323396	24.5412	PPB	96
14) Propylene oxide	3.12	58	1922	1.1917	PPB	# 13
15) Iodomethane	3.13	142	358397	17.8318	PPB	93
16) Bromoethane	3.25	108	224334	20.2220	PPB	100
17) Acrolein	3.34	56	99705	127.3557	PPB	99
18) 3-Chloropropene	3.48	41	694663	25.0757	PPB	92
19) Methylene chloride	3.59	84	291476	18.6709	PPB	88
20) Acetone	3.65	58	11301	16.7653	PPB	# 75
21) trans-1,2-Dichloroethene	3.75	96	342388	22.3284	PPB	93
22) Methyl acetate	3.77	74	56602	48.4189	PPB	# 76
23) Hexane	3.83	86	128785	25.1847	PPB	# 73
24) Methyl tert-butyl ether (M)	3.86	73	588143	18.4611	PPB	# 75
25) tert-Butyl alcohol	3.98	59	219607	354.7499	PPB	90
26) Acetonitrile	4.11	40	50154	91.0416	PPB	92
27) Isopropyl ether	4.25	45	1275894	22.6538	PPB	95
28) 2-Chloro-1,3-butadiene	4.36	88	284166	24.0450	PPB	# 76
29) 1,1-Dichloroethane (SPCC)	4.38	63	667498	22.2169	PPB	99
30) Acrylonitrile	4.43	53	270452	94.4088	PPB	99
31) Vinyl acetate	4.65	43	411117	22.6213	PPB	95
32) cis-1,2-Dichloroethene	4.94	96	329507	20.3884	PPB	93
33) 2,2-Dichloropropane	5.05	77	498928	22.1453	PPB	85
34) Cyclohexane	5.14	56	760178	27.1682	PPB	90
35) Bromochloromethane	5.15	130	139602	18.4432	PPB	# 84
37) Chloroform (CCC)	5.24	83	533845	20.5780	PPB	97
38) Carbon tetrachloride	5.37	117	418198	23.8307	PPB	99
41) Tetrahydrofuran	5.39	72	20605	19.6369	PPB	90
43) 1,1,1-Trichloroethane	5.43	97	491254	22.6438	PPB	96
44) 1,1-Dichloropropene	5.57	75	511778	24.5412	PPB	86
45) 2-Butanone (MEK)	5.56	43	58917	17.8609	PPB	98
46) Benzene	5.84	78	1458611	22.1988	PPB	96

(#)=qualifier out of range (m)=manual integration (s)=analyte in sublist
 I126907.D I81104W.M Tue Jan 27 13:50:03 2009 RPT1

Data File : H:\MSI.I\I012609.B\I126907.D Vial: 7
 Acq On : 26 Jan 2009 8:48 am Operator: DY
 Sample : BATCH-MSD1@1X MSD,REGC Inst : MSI
 Misc : 9010191 4.2uL/42mL; VIALS 1-J,M,Q;G Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:48 19109 Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
48) Propanenitrile	5.87	54	102174	94.8949	PPB	98
49) Methacrylonitrile	5.89	67	325400	94.0127	PPB #	80
51) 1,2-Dichloroethane	6.06	62	336245	21.2106	PPB	99
52) Isobutyl alcohol	6.13	43	101438	320.4111	PPB	97
53) Methylcyclohexane	6.47	83	1285562	65.1088	PPB	93
54) Trichloroethene	6.49	130	327079	21.4780	PPB	95
55) Dibromomethane	6.96	93	108676	19.0047	PPB	93
56) n-Butanol	6.92	56	110648	553.7626	PPB	85
57) 1,2-Dichloropropane (CCC)	7.08	63	333116	21.6701	PPB	92
58) Bromodichloromethane	7.17	83	367397	20.8344	PPB	97
59) 1,4-Dioxane	7.41	88	25137	366.3809	PPB	92
60) Methyl methacrylate	7.36	69	99661	16.3839	PPB	80
61) 1-Bromo-2-chloroethane	7.71	63	313975	19.3334	PPB	99
62) cis-1,3-Dichloropropene	7.90	75	457852	21.0747	PPB	88
66) Toluene (CCC)	8.13	91	1442176	20.0629	PPB	97
67) Epichlorohydrin	8.16	57	52306	71.3900	PPB	82
68) 2-Nitropropane	8.37	43	31464	17.4285	PPB	95
69) Tetrachloroethene	8.50	164	229228	19.2693	PPB	98
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	139210	19.2043	PPB	95
71) trans-1,3-Dichloropropene	8.54	75	343582	18.5534	PPB	88
72) 1,1,2-Trichloroethane	8.68	97	162178	16.5478	PPB	96
73) 4-Methyl-2-pentanol (MIBC)	8.62	45	67443	48.1046	PPB	87
74) Ethyl methacrylate	8.69	69	218335	16.2201	PPB	82
75) Dibromochloromethane	8.83	129	196487	18.5884	PPB	99
76) 1,3-Dichloropropane	8.91	76	343775	17.2669	PPB	87
77) 1,2-Dibromoethane (EDB)	9.02	107	146857	16.9492	PPB	98
78) 2-Hexanone	9.21	43	78813	17.6895	PPB	92
79) Chlorobenzene (SPCC)	9.44	112	874983	19.7526	PPB	94
80) 1-Chlorohexane	9.43	55	420256	25.9180	PPB	92
81) Ethylbenzene (CCC)	9.46	106	526175	20.9485	PPB	96
82) 1,1,1,2-Tetrachloroethane	9.49	131	260256	19.1955	PPB	99
83) m&p-Xylene	9.57	106	1304010	41.8956	PPB	96
84) o-Xylene	9.88	106	600454	20.8205	PPB	96
85) Bromoform (SPCC)	9.94	173	87628	18.5439	PPB	100
86) Styrene	9.91	104	922521	21.5964	PPB	97
87) Isopropylbenzene	10.09	105	1567552	23.0640	PPB	98
88) Bromobenzene	10.36	156	286286	19.7991	PPB #	87
89) n-Propylbenzene	10.37	120	402594	20.9010	PPB #	88
90) 1,1,2,2-Tetrachloroethane	10.43	83	176952	17.4137	PPB	99
93) 2-Chlorotoluene	10.48	126	348325	20.4392	PPB	89
95) 1,2,3-Trichloropropane	10.51	110	51636	14.6837	PPB	98
96) trans-1,4-Dichloro-2-buten	10.54	53	49693	19.0821	PPB	82
97) 3-Ethyltoluene	10.43	105	1526530	21.0452	PPB	98
98) 4-Chlorotoluene	10.59	126	343021	20.3021	PPB	91
99) 1,3,5-Trimethylbenzene	10.50	105	1235717	20.1726	PPB	68
100) 2-Ethyltoluene	10.64	105	1498376	20.3792	PPB	76
101) tert-Butylbenzene	10.70	91	714488	21.2508	PPB	90
103) 1,2,4-Trimethylbenzene	10.75	105	1227268	20.0067	PPB	98
104) sec-Butylbenzene	10.81	105	1661709	22.2078	PPB	97
105) p-Isopropyltoluene	10.90	119	1337501	20.9151	PPB	97
106) 1,3-Dichlorobenzene	10.96	146	593166	19.5396	PPB	99
107) 1,4-Dichlorobenzene	11.01	146	602031	18.7330	PPB	99
108) Benzyl chloride	11.16	126	51472	14.1147	PPB #	27
109) n-Butylbenzene	11.16	134	311417	20.8609	PPB	90
110) 1,2-Dichlorobenzene	11.27	146	472426	18.7114	PPB	99

(#)=qualifier out of range (m)=manual integration (s)=analyte in sublist
 I126907.D I81104W.M Tue Jan 27 13:50:04 2009 RPT1

Data File : H:\MSI.I\I012609.B\I126907.D Vial: 7
 Acq On : 26 Jan 2009 8:48 am Operator: DY
 Sample : BATCH-MSD1@1X MSD,REGC Inst : MSI
 Misc : 9010191 4.2uL/42mL; VIALS 1-J,M,Q;G Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:48 19109 Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
112) 1,2-Dibromo-3-chloropropan	11.75	157	17735	13.1620	PPB	91
113) Hexachlorobutadiene	12.11	225	155288	20.2714	PPB	99
114) 1,2,4-Trichlorobenzene	12.13	180	284596	21.1077	PPB	100
115) Naphthalene	12.32	128	416706	21.2539	PPB	100
116) 1,2,3-Trichlorobenzene	12.43	180	191011	19.9502	PPB	99


Quantitation Report

Data File : H:\MSI.I\I012609.B\I126907.D
Acq On : 26 Jan 2009 8:48 am
Sample : BATCH-MSD1@1X MSD,REGC
Misc : 9010191 4.2uL/42mL; VIALS 1-J,M,Q;G
MS Integration Params: VOA.P
Quant Time: Jan 27 12:48 19109

vial: 7
Operator: DY
Inst : MSI
Multiplr: 1.00



Quant Results File: I81104W.RES

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL water
Last Update : Tue Nov 11 14:35:13 2008
Response via : Initial Calibration

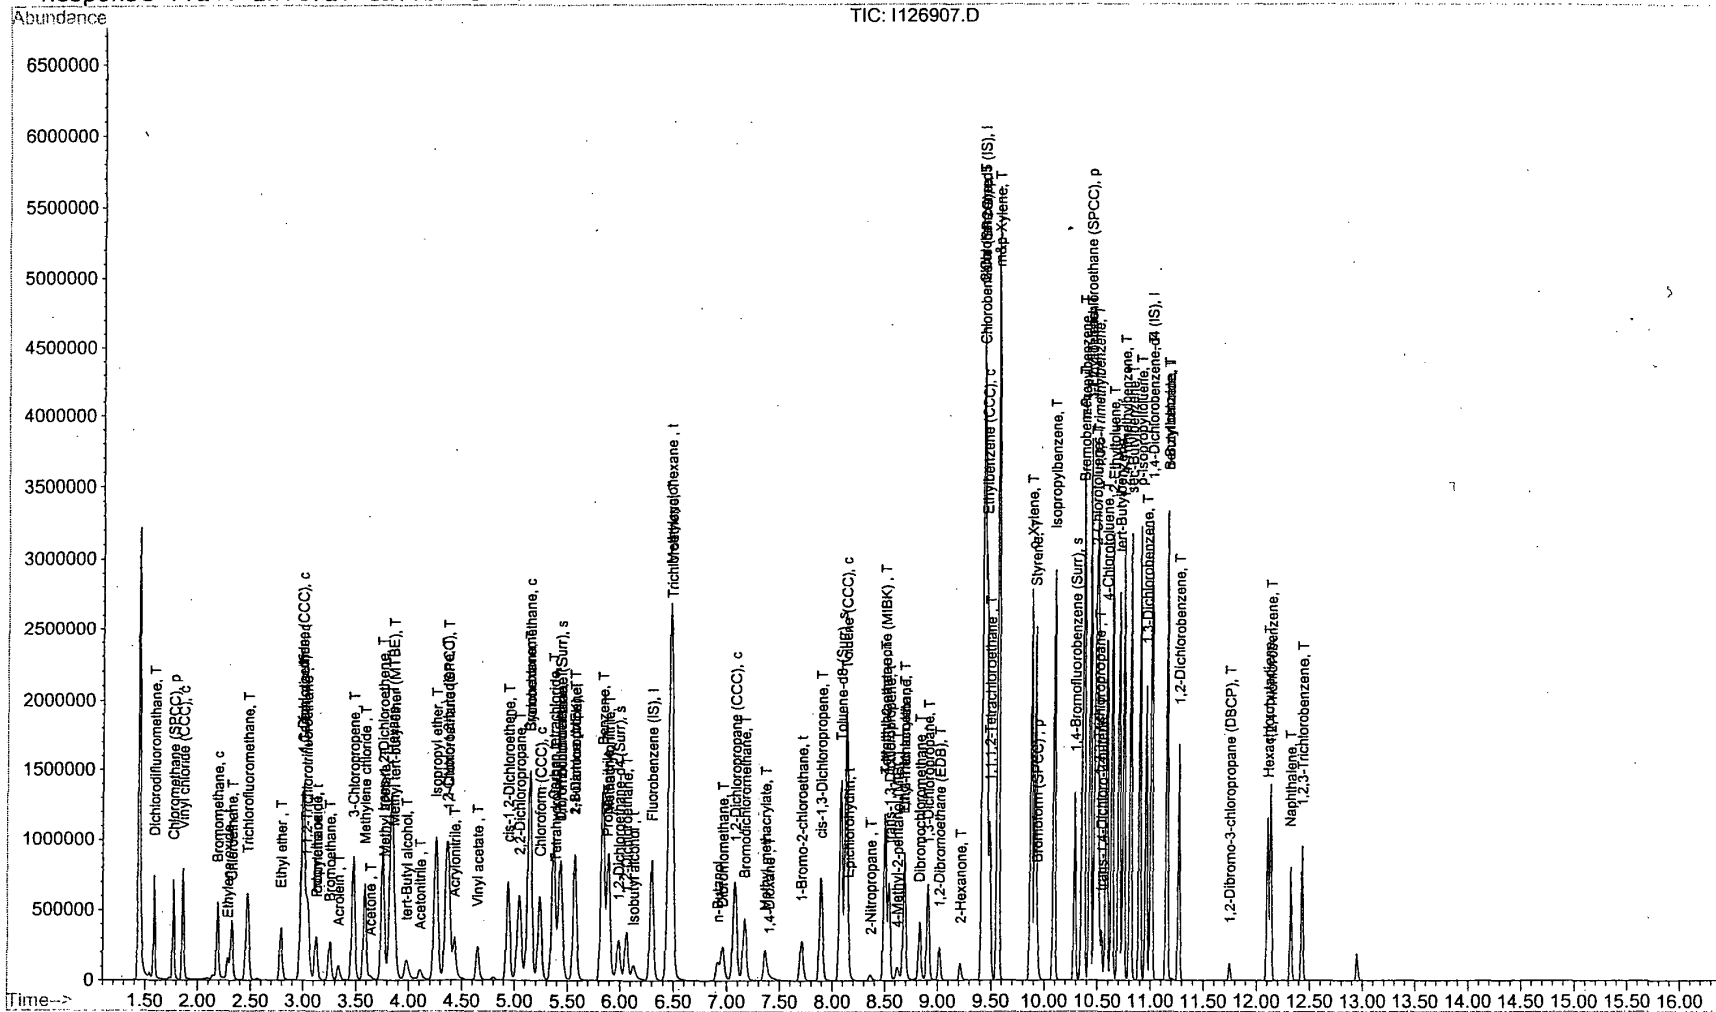

BFB

Data File : H:\MSI.I\I012609.B\I126908.D Vial: 8
 Acq On : 26 Jan 2009 9:15 am Operator: DY
 Sample : CCV,REG Inst : MSI
 Misc : 9010191 5uL/50mL Multiplr: 1.00
 MS Integration Params: VOA.P
 Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water

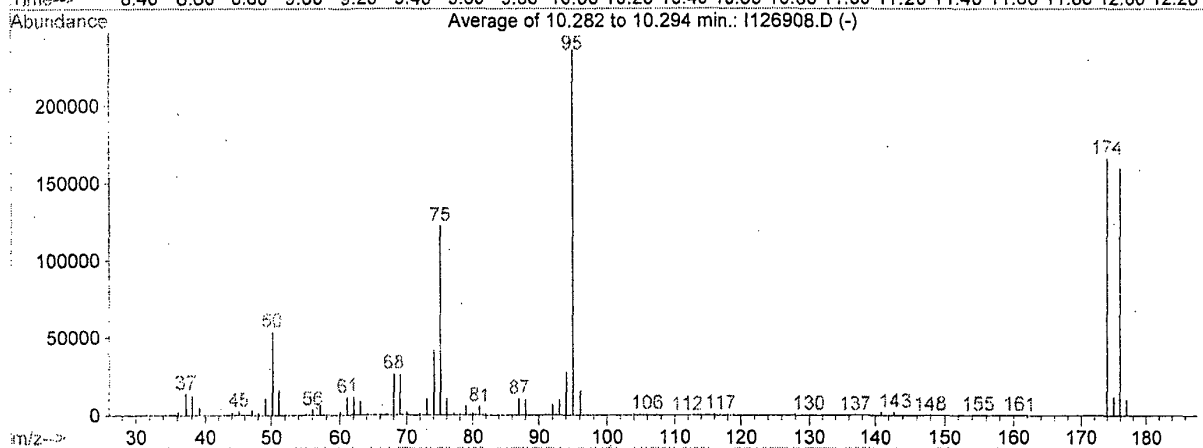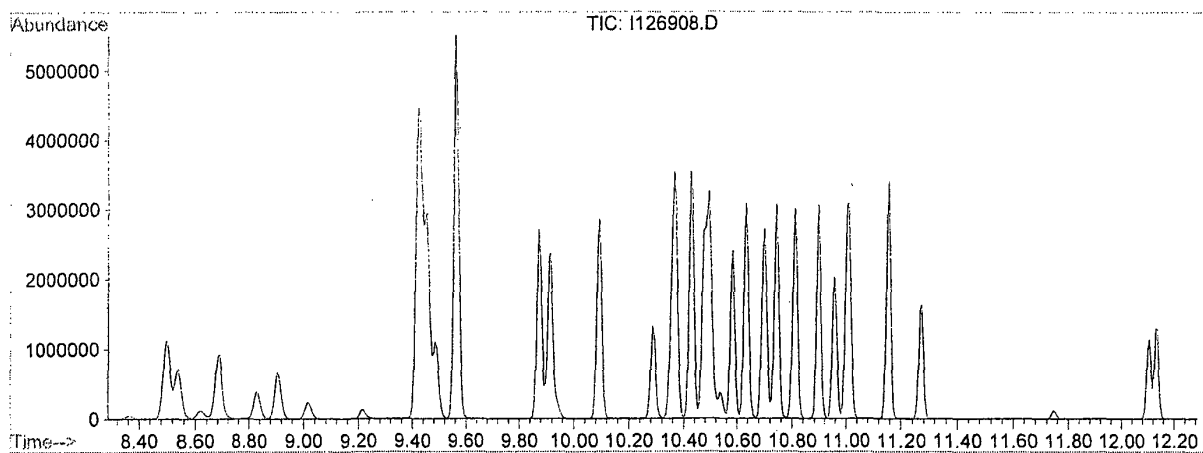

AutoFind: Scans 1511, 1512, 1513; Background Corrected with Scan 1505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	54027	PASS
75	95	30	60	51.8	122221	PASS
95	95	100	100	100.0	235819	PASS
96	95	5	9	6.8	15953	PASS
173	174	0.00	2	0.2	360	PASS
174	95	50	100	70.5	166221	PASS
175	174	5	9	7.0	11654	PASS
176	174	95	101	96.4	160245	PASS
177	176	5	9	6.4	10335	PASS

I126908.D I81104W.M Mon Jan 26 09:37:09 2009 MSI

MSI
1/26/09

Quantitation Report (QI Reviewed)

1-29-09 48/132

Data File : H:\MSI.I\I012609.B\I126908.D
 Acq On : 26 Jan 2009 9:15 am
 Sample : CCV,REGC
 Misc : 9010191 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:59 19109

Vial: 8
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

JAN 27 2009

Only worked up
 Target Analytes

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	924953	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	216076	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.01	152	300940	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	224719	16.6571	PPB	0.00
Spiked Amount	16.700		Recovery	=	99.76%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	125694	16.3301	PPB	0.00
Spiked Amount	16.700		Recovery	=	97.78%	
64) Toluene-d8 (Surr)	8.08	98	973973	18.3399	PPB	0.00
Spiked Amount	16.700		Recovery	=	109.82%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	348975	17.2781	PPB	0.00
Spiked Amount	16.700		Recovery	=	103.47%	
Target Compounds						
2) Dichlorodifluoromethane	1.59	85	402734	19.7026	PPB	S 98
3) Chloromethane (SPCC)	1.77	50	443172	22.1112	PPB	S 99
4) Vinyl chloride (CCC)	1.86	62	482697	22.2761	PPB	S 100
5) Bromomethane	2.18	94	267810	23.7007	PPB	S 99
6) Ethylene oxide	2.28	44	395624	239.7384	PPB	99
7) Chloroethane	2.32	64	319861	21.8516	PPB	97
8) Trichlorofluoromethane	2.47	101	499976	22.2645	PPB	99
9) Ethyl ether	2.79	59	220867	19.2074	PPB	92
11) 1,1-Dichloroethene (CCC)	2.99	96	282209	20.3441	PPB	90
12) Carbon disulfide	3.01	76	1076929	22.0713	PPB	96
13) 1,1,2-Trichlorotrifluoroet	3.04	101	299960	22.4254	PPB	96
14) Propylene oxide	3.12	58	148211	90.5342	PPB	91
15) Iodomethane	3.13	142	352611	17.3169	PPB	93
16) Bromoethane	3.25	108	222853	19.7908	PPB	100
17) Acrolein	3.33	56	104251	131.1886	PPB	100
18) 3-Chloropropene	3.47	41	670219	23.8347	PPB	92
19) Methylene chloride	3.58	84	290454	18.3297	PPB	89
20) Acetone	3.64	58	12258	17.9154	PPB	# 81
21) trans-1,2-Dichloroethene	3.75	96	327479	21.0395	PPB	93
22) Methyl acetate	3.77	74	59108	49.8132	PPB	# 68
23) Hexane	3.83	86	118222	22.7764	PPB	# 71
24) Methyl tert-butyl ether (M	3.86	73	603998	18.6778	PPB	87
25) tert-Butyl alcohol	3.99	59	249372	396.8609	PPB	90
26) Acetonitrile	4.11	40	49870	89.1842	PPB	92
27) Isopropyl ether	4.26	45	1272913	22.2658	PPB	95
28) 2-Chloro-1,3-butadiene	4.36	88	269091	22.4319	PPB	# 78
29) 1,1-Dichloroethane (SPCC)	4.38	63	643479	21.1000	PPB	100
30) Acrylonitrile	4.43	53	276908	95.2297	PPB	98
31) vinyl acetate	4.65	43	431725	23.4031	PPB	95
32) cis-1,2-Dichloroethene	4.94	96	322236	19.6430	PPB	93
33) 2,2-Dichloropropane	5.04	77	472690	20.6697	PPB	86
34) Cyclohexane	5.14	56	700689	24.6709	PPB	90
35) Bromochloromethane	5.15	130	142190	18.5067	PPB	84
37) Chloroform (CCC)	5.24	83	510946	19.4034	PPB	98
38) Carbon tetrachloride	5.37	117	397911	22.3386	PPB	100
41) Tetrahydrofuran	5.40	72	20822	19.5496	PPB	# 85
43) 1,1,1-Trichloroethane	5.44	97	466055	21.1638	PPB	97
44) 1,1-Dichloropropene	5.57	75	482618	22.7999	PPB	87
45) 2-Butanone (MEK)	5.56	43	64735	19.3338	PPB	88
46) Benzene	5.83	78	1412955	21.1852	PPB	96

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 I126908.D I81104W.M Tue Jan 27 13:50:23 2009 RPT1

Data File : H:\MSI.I\I012609.B\I126908.D
 Acq On : 26 Jan 2009 9:15 am
 Sample : CCV,REGC
 Misc : 9010191 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:59 19109

Vial: 8
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
48) Propanenitrile	5.87	54	104091	95.2424	PPB	87
49) Methacrylonitrile	5.89	67	337678	96.1139	PPB	82
51) 1,2-Dichloroethane	6.07	62	339242	21.0825	PPB	99
52) Isobutyl alcohol	6.13	43	114690	354.6349	PPB	96
53) Methylcyclohexane	6.47	83	1196221	59.6860	PPB	93
54) Trichloroethene	6.49	130	315745	20.4264	PPB	96
55) Dibromomethane	6.97	93	111286	19.1727	PPB	93
56) n-Butanol	6.92	56	135497	655.6476	PPB	88
57) 1,2-Dichloropropane (CCC)	7.08	63	330064	21.1533	PPB	92
58) Bromodichloromethane	7.17	83	355164	19.8422	PPB	98
59) 1,4-Dioxane	7.40	88	29713	426.6585	PPB	92
60) Methyl methacrylate	7.37	69	103538	16.7511	PPB	79
61) 1-Bromo-2-chloroethane	7.71	63	319145	19.3604	PPB	98
62) cis-1,3-Dichloropropene	7.90	75	469591	21.2947	PPB	88
63) 2-Chloroethyl vinyl ether	7.84	63	91065	19.6008	PPB	94
66) Toluene (CCC)	8.13	91	1402109	19.2214	PPB	98
67) Epichlorohydrin	8.16	57	62086	83.5037	PPB	96
68) 2-Nitropropane	8.37	43	33800	18.4497	PPB	95
69) Tetrachloroethene	8.50	164	221453	18.3446	PPB	98
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	144597	19.6569	PPB	94
71) trans-1,3-Dichloropropene	8.54	75	348409	18.5400	PPB	88
72) 1,1,2-Trichloroethane	8.68	97	166145	16.7056	PPB	96
73) 4-Methyl-2-pentanol (MIBC)	8.62	45	83984	57.0332	PPB	89
74) Ethyl methacrylate	8.69	69	227803	16.6664	PPB	83
75) Dibromochloromethane	8.83	129	193779	18.0651	PPB	99
76) 1,3-Dichloropropane	8.91	76	352024	17.4236	PPB	88
77) 1,2-Dibromoethane (EDB)	9.02	107	150105	17.0716	PPB	100
78) 2-Hexanone	9.22	43	83332	18.4313	PPB	94
79) Chlorobenzene (SPCC)	9.44	112	864765	19.2375	PPB	96
80) 1-Chlorohexane	9.42	55	389354	23.5288	PPB	91
81) Ethylbenzene (CCC)	9.45	106	507995	19.9301	PPB	93
82) 1,1,1,2-Tetrachloroethane	9.48	131	260871	18.9606	PPB	99
83) m&p-xylene	9.56	106	1274208	40.3417	PPB	96
84) o-xylene	9.87	106	590640	20.1818	PPB	96
85) Bromoform (SPCC)	9.94	173	87666	18.2817	PPB	100
86) Styrene	9.92	104	918205	21.1822	PPB	96
87) Isopropylbenzene	10.09	105	1519721	22.0345	PPB	98
88) Bromobenzene	10.36	156	288953	19.6924	PPB	# 88
89) n-Propylbenzene	10.37	120	390038	19.9541	PPB	89
90) 1,1,2,2-Tetrachloroethane	10.43	83	183615	17.8062	PPB	98
93) 2-Chlorotoluene	10.48	126	341166	19.5169	PPB	90
95) 1,2,3-Trichloropropane	10.51	110	54611	15.1401	PPB	99
96) trans-1,4-Dichloro-2-buten	10.54	53	54770	20.5041	PPB	83
97) 3-Ethyltoluene	10.43	105	1484463	19.9518	PPB	98
98) 4-Chlorotoluene	10.59	126	338777	19.5479	PPB	94
99) 1,3,5-Trimethylbenzene	10.49	105	1204781	19.1742	PPB	68
100) 2-Ethyltoluene	10.63	105	1465372	19.4303	PPB	76
101) tert-Butylbenzene	10.70	91	685957	19.8904	PPB	90
103) 1,2,4-Trimethylbenzene	10.74	105	1210290	19.2350	PPB	98
104) sec-Butylbenzene	10.81	105	1582697	20.6212	PPB	98
105) p-Isopropyltoluene	10.90	119	1288641	19.6455	PPB	97
106) 1,3-Dichlorobenzene	10.96	146	586946	18.8497	PPB	99
107) 1,4-Dichlorobenzene	11.01	146	597806	18.1349	PPB	99
108) Benzyl chloride	11.16	126	55300	14.6356	PPB	# 46
109) n-Butylbenzene	11.16	134	300190	19.6044	PPB	89

(#)=qualifier out of range (m)=manual integration (s)=analyte in sublist
 I126908.D I81104W.M Tue Jan 27 13:50:23 2009 RPT1

Data File : H:\MSI.I\I012609.B\I126908.D Vial: 8
 Acq On : 26 Jan 2009 9:15 am Operator: DY
 Sample : CCV,REGC Inst : MSI
 Misc : 9010191 5uL/50mL Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:59 19109 Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
110) 1,2-Dichlorobenzene	11.27	146	475901	18.3761	PPB	99
112) 1,2-Dibromo-3-chloropropan	11.75	157	17858	12.9459	PPB	91
113) Hexachlorobutadiene	12.11	225	149069	18.9714	PPB	100
114) 1,2,4-Trichlorobenzene	12.14	180	288083	20.8302	PPB	100
115) Naphthalene	12.33	128	431962	21.4793	PPB	100
116) 1,2,3-Trichlorobenzene	12.43	180	194628	19.8180	PPB	99


Quantitation Report

Data File : H:\MSI.I\I012609.B\I126908.D
 Acq On : 26 Jan 2009 9:15 am
 Sample : CCV,REGC
 Misc : 9010191 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 12:59 19109

Via: 8
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:35:13 2008
 Response via : Initial Calibration

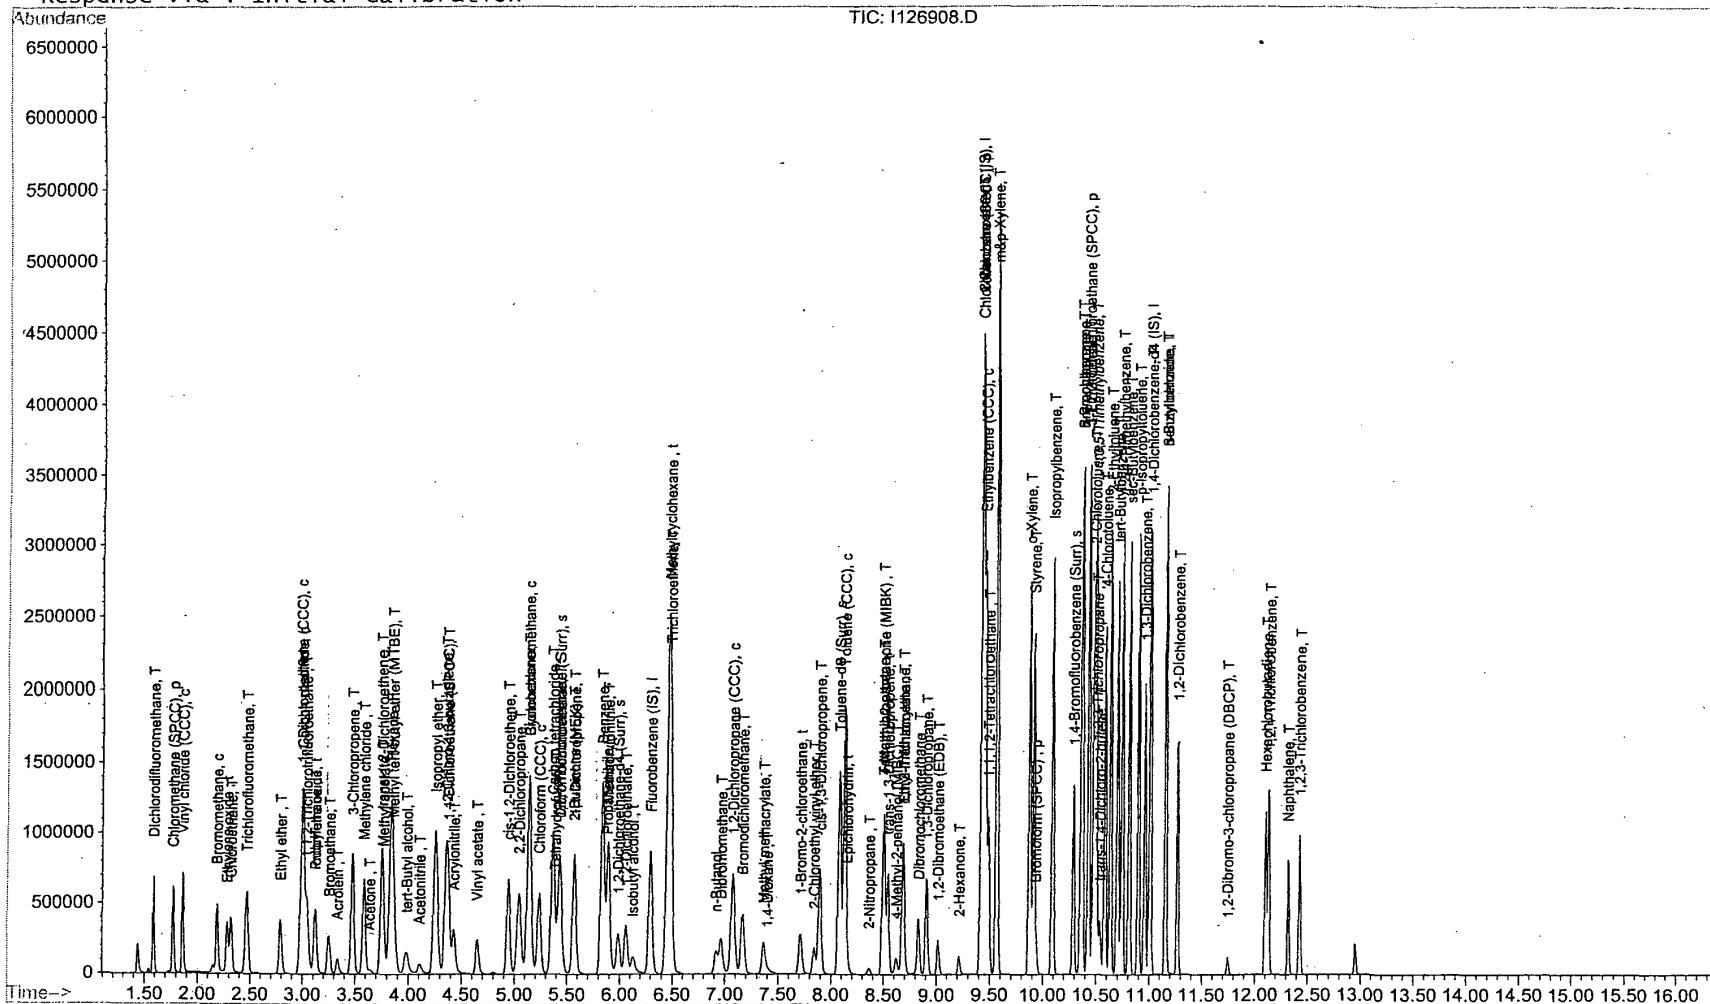

QUANTIFICATION REPORT (QI Reviewed)

52/132

Data File : H:\MSI.I\I012609.B\I126911.D
 Acq On : 26 Jan 2009 10:37 am
 Sample : BATCH-BLK1@1,REGC
 Misc : 1,1, 9010225 5uL/50mL
 MS Integration Params: VOA.P
 Quant Time: Jan 27 13:09 19109

Vial: 11
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

1-29-09

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:49:50 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

JS JAN 27 2009

**Only worked up:
 Target Analytes**

Internal standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	864731	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	186995	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.00	152	252378	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	198093	15.7061	PPB	0.00
Spiked Amount	16.700		Recovery	=	94.07%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	110828	15.4015	PPB	0.00
Spiked Amount	16.700		Recovery	=	92.22%	
64) Toluene-d8 (Surr)	8.08	98	892663	17.9795	PPB	0.00
Spiked Amount	16.700		Recovery	=	107.66%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	305942	17.5032	PPB	0.00
Spiked Amount	16.700		Recovery	=	104.79%	
Target Compounds						
5) Bromomethane	2.19	94	2670	0.2527	PPB	Qvalue S 97
6) Ethylene oxide	2.25	44	4407	2.8565	PPB	83
10) Ethanol	2.88	45	419	5.6776	PPB	# 19

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 I126911.D I81104W.M Tue Jan 27 13:50:42 2009 RPT1


Quantitation Report

Data File : H:\MSI.I\I012609.B\I126911.D
Acq On : 26 Jan 2009 10:37 am
Sample : BATCH-BLK1@1,REGC
Misc : 1,1, 9010225 5uL/50mL
MS Integration Params: VOA.P
Quant Time: Jan 27 13:09 19109

Vial: 11
Operator: DY
Inst : MSI
Multiplr: 1.00

Quant Results File: I81104W.RES

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Tue Nov 11 14:35:13 2008
Response via : Initial Calibration

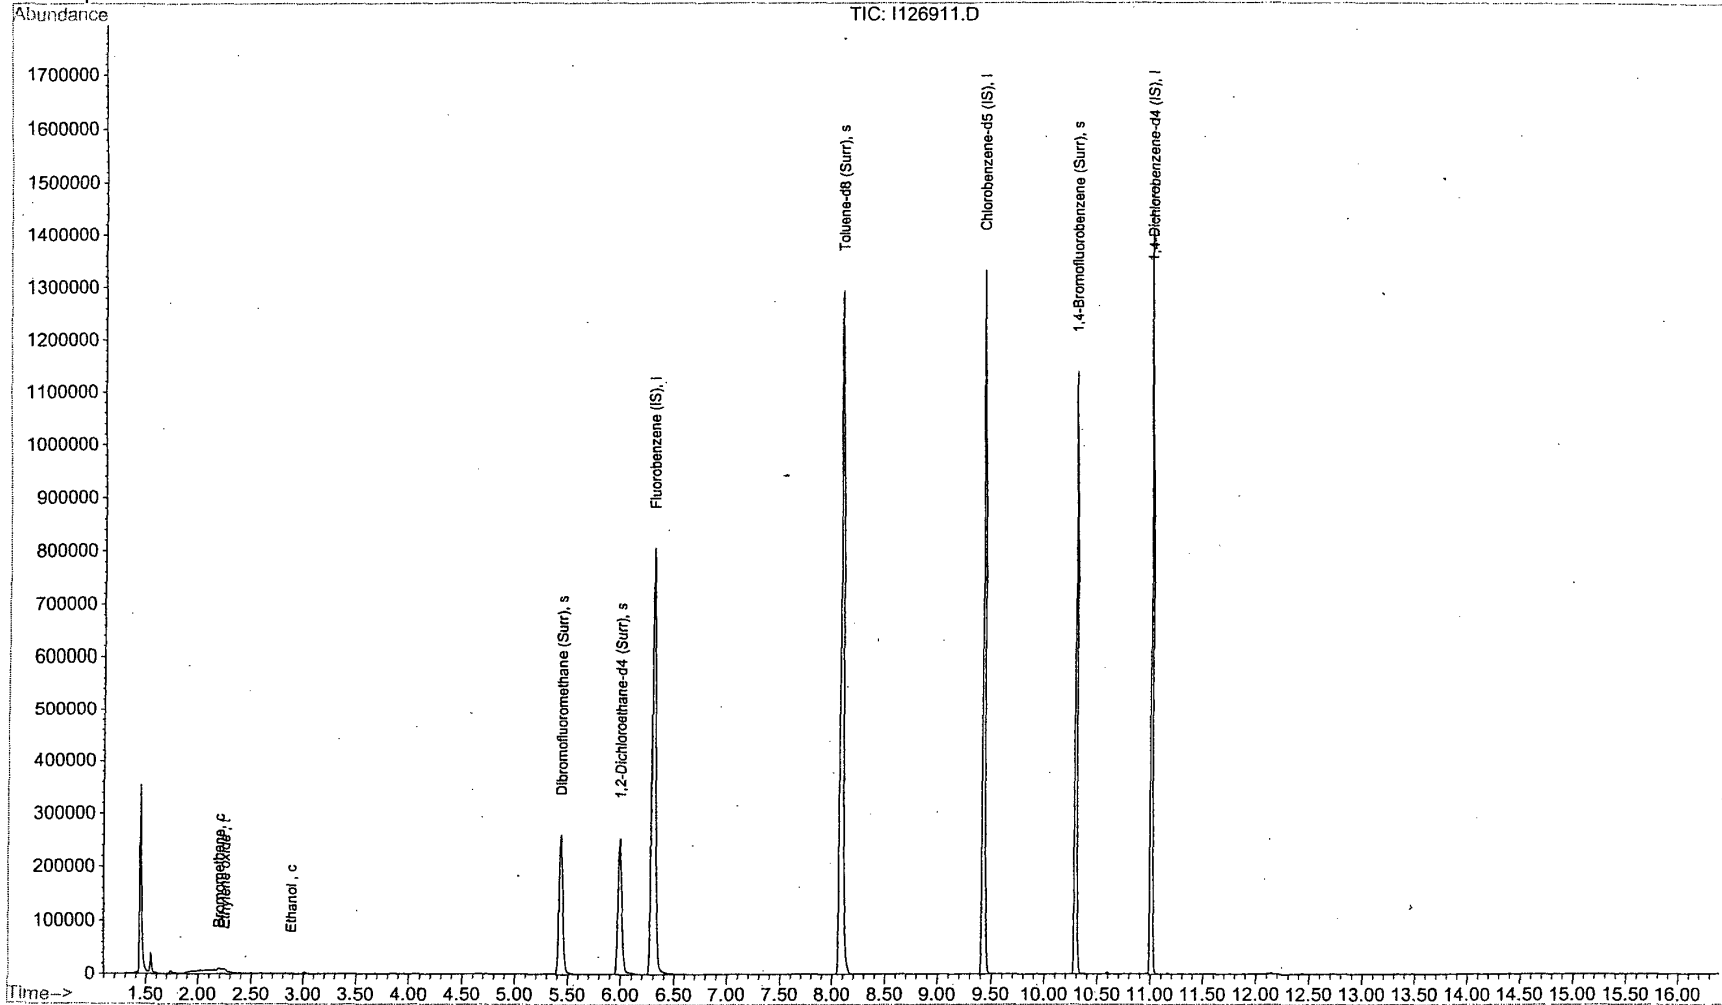

Quantitation Report (QI Reviewed)

Data File : H:\MSI.I\I012609.B\I126912.D
 Acq On : 26 Jan 2009 11:04 am
 Sample : ASA0148-01 001X ,REGC
 Misc : VIALS 1-J,M,Q;G
 MS Integration Params: VOA.P
 Quant Time: Jan 27 13:10 19109

vial: 12
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

1-29-9mm 54/132

Parent

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:49:50 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

53

JAN 27 2009

Only worked up:
 Target Analytes

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	830237	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	174391	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.00	152	229035	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	207593	17.1431	PPB	0.00
Spiked Amount	16.700		Recovery	=	102.63%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	110623	16.0117	PPB	0.00
Spiked Amount	16.700		Recovery	=	95.87%	
64) Toluene-d8 (Surr)	8.08	98	853383	17.9025	PPB	0.00
Spiked Amount	16.700		Recovery	=	107.19%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	288027	17.6692	PPB	0.00
Spiked Amount	16.700		Recovery	=	105.81%	
Target Compounds						
5) Bromomethane	2.20	94	2358	0.2325	PPB	Qvalue S 91
6) Ethylene oxide	2.26	44	4185	2.8253	PPB	74
20) Acetone	3.65	58	546	0.8890	PPB	# 11
37) Chloroform (CCC)	5.24	83	11091	0.4692	PPB	96
58) Bromodichloromethane	7.17	83	7938	0.4941	PPB	93
75) Dibromochloromethane	8.83	129	6968	0.8049	PPB	98
85) Bromoform (SPCC)	9.94	173	2260	0.5839	PPB	98


Quantitation Report

Data File : H:\MSI.I\I012609.B\I126912.D
Acq On : 26 Jan 2009 11:04 am
Sample : ASA0148-01 0@1X ,REGC
Misc : VIALS 1-J,M,Q;G
MS Integration Params: VOA.P
Quant Time: Jan 27 13:10 19109

Vial: 12
Operator: DY
Inst : MSI
Multiplr: 1.00

Quant Results File: I81104W.RES

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Tue Nov 11 14:35:13 2008
Response via : Initial Calibration

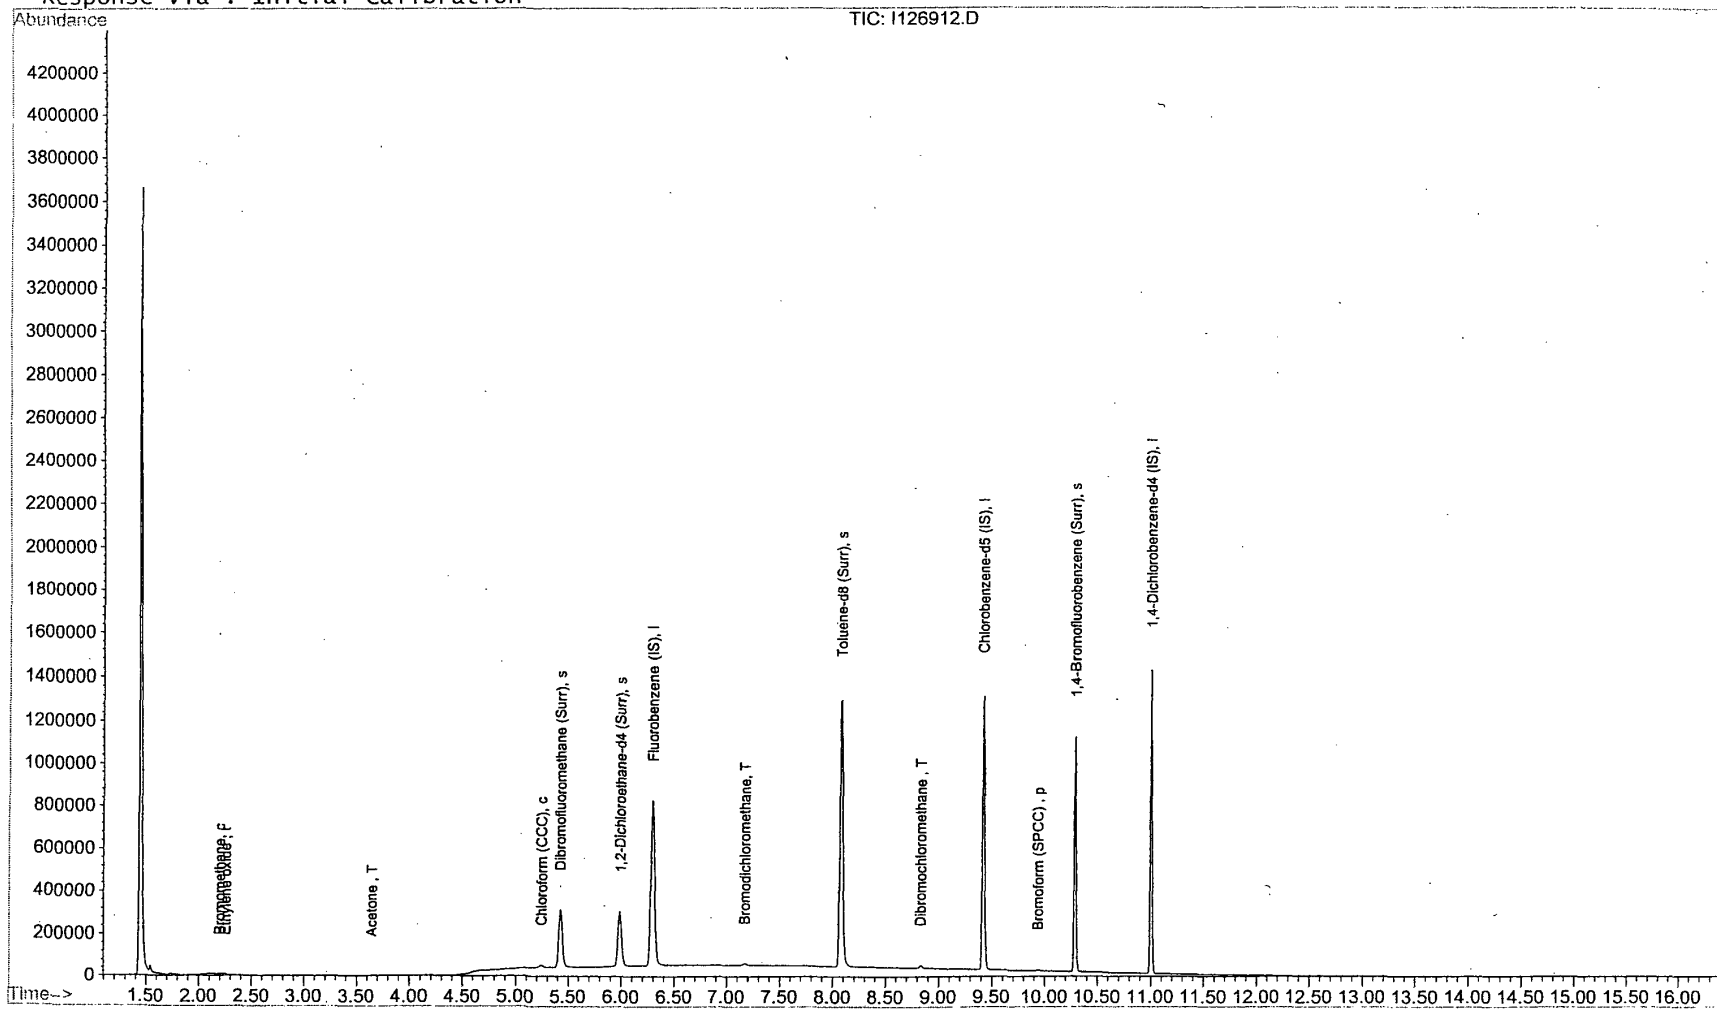

Data File : H:\MSI.I\I012609.B\I126913.D Vial: 13
 Acq On : 26 Jan 2009 11:32 am Operator: DY
 Sample : ASA0086-01 @1X A,REGC Only worked up: Target Analytes Inst : MSI
 Misc : Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Jan 29 13:56 19109 Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:49:50 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

CIS ↑ RR data file 32

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.30	96	786284	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	171658	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.00	152	233481	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	191791	16.7235	PPB	0.00
Spiked Amount				16.700		
				Recovery	=	100.12%
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	110444	16.8794	PPB	0.00
Spiked Amount				16.700		
				Recovery	=	101.08%
64) Toluene-d8 (Surr)	8.08	98	819113	18.1441	PPB	0.00
Spiked Amount				16.700		
				Recovery	=	108.62%
91) 1,4-Bromofluorobenzene (Su)	10.29	95	291544	18.1697	PPB	0.00
Spiked Amount				16.700		
				Recovery	=	108.80%
Target Compounds						
4) Vinyl chloride (CCC)	1.86	62	5839	0.3170	PPB	Qvalue # S 1
5) Bromomethane	2.19	94	2934	0.3054	PPB	S 98
11) 1,1-Dichloroethene (CCC)	2.99	96	17221	1.4604	PPB	88
12) Carbon disulfide	3.00	76	47447m	1.1439	PPB	
20) Acetone	3.65	58	569	0.9783	PPB	# 23
21) trans-1,2-Dichloroethene	3.75	96	7024	0.5309	PPB	92
29) 1,1-Dichloroethane (SPCC)	4.38	63	588627	22.7053	PPB	100
32) cis-1,2-Dichloroethene	4.94	96	1741037	124.8479	PPB	93
43) 1,1,1-Trichloroethane	5.44	97	14253	0.7614	PPB	94
46) Benzene	5.83	78	86547	1.5265	PPB	96
51) 1,2-Dichloroethane	6.07	62	7945	0.5808	PPB	97
54) Trichloroethene	6.49	130	473074	36.0019	PPB	95
57) 1,2-Dichloropropane (CCC)	7.08	63	3820	0.2880	PPB	79
66) Toluene (CCC)	8.13	91	44668	0.7708	PPB	98
69) Tetrachloroethene	8.50	164	4980	0.5193	PPB	96
87) Isopropylbenzene	10.10	105	14251	0.2601	PPB	97
95) 1,2,3-Trichloropropane	10.51	110	14960	5.3457	PPB	99

Only worked up:
Target Analytes


Quantitation Report

Data File : H:\MSI.I\I012609.B\I126913.D
Acq On : 26 Jan 2009 11:32 am
Sample : ASA0086-01 @1X A,REGC
Misc :
MS Integration Params: VOA.P
Quant Time: Jan 29 13:56 19109

Vial: 13
Operator: DY
Inst : MSI
Multiplr: 1.00

Quant Results File: I81104W.RES

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Tue Nov 11 14:35:13 2008
Response via : Initial Calibration

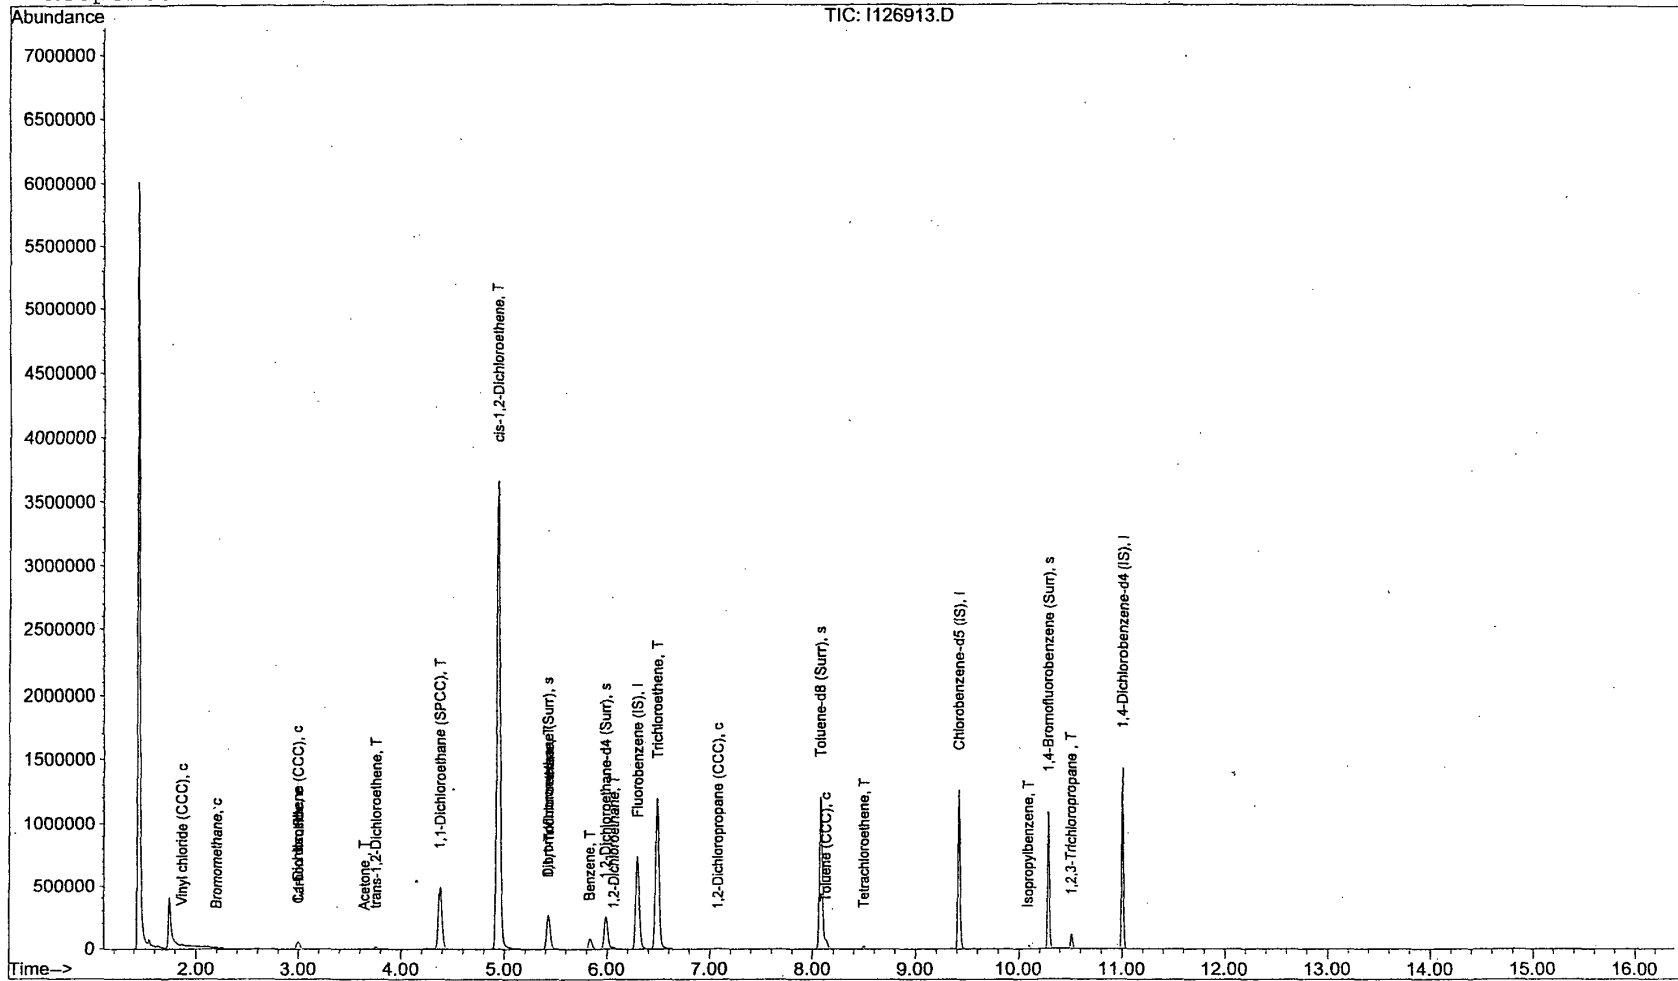

Carbon disulfide

I126913.D


1-29-09

REASON FOR MANUAL INTEGRATION:

TAILING WRONG PEAK TWO PEAKS POOR INTEGRATION MISSED OTHER

ANALYST: DY Thu Jan 29 13:56:22 2009

BEFORE

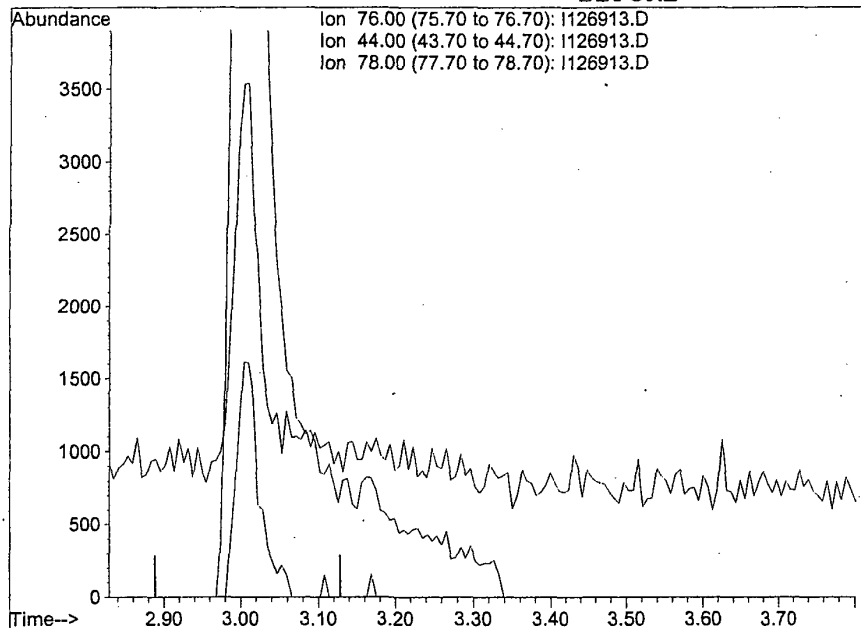

TIC: I126913.D


(12) Carbon disulfide (c)

3.01min 0.00PPB d

response 0

Ion	Exp%	Act%
76.00	100	0.00
44.00	12.50	0.00
78.00	9.70	0.00
0.00	0.00	0.00

AFTER

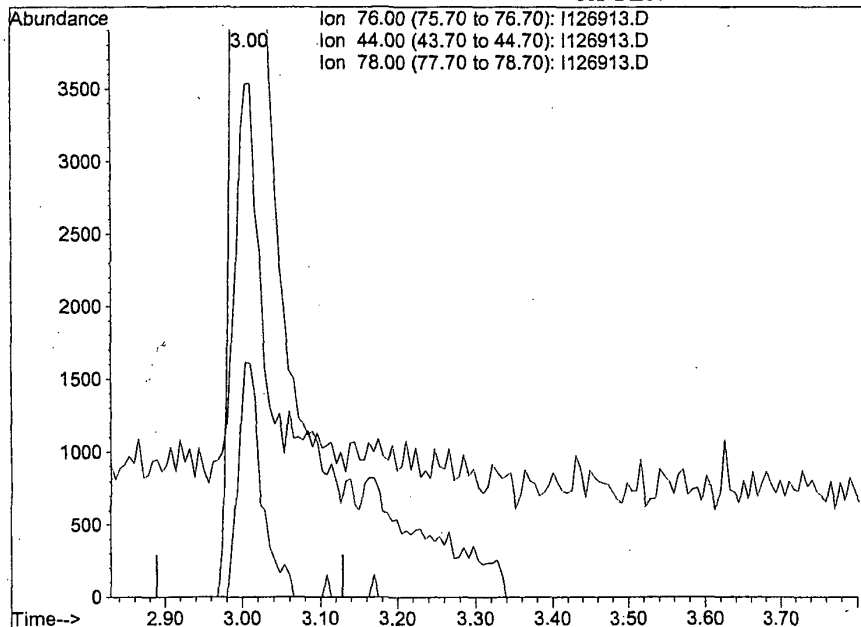

TIC: I126913.D

(12) Carbon disulfide (c)

3.00min 1.14PPB m

response 47447

Ion	Exp%	Act%
76.00	100	100
44.00	12.50	13.24
78.00	9.70	7.09
0.00	0.00	0.00

1/30/09

Data File : H:\MSI.I\I012609.B\I126914.D
 Acq On : 26 Jan 2009 11:59 am
 Sample : ASA0086-02 @1X A,REGC
 Misc :
 MS Integration Params: VOA.P
 Quant Time: Jan 27 13:39 19109

Vial: 14
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

1-29-913

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:49:50 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

SB JAN 27 2009

**Only worked up:
 Target Analytes**

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	771905	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	171111	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.00	152	231332	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	189055	16.7920	PPB	0.00
Spiked Amount	16.700		Recovery	=	100.54%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	110807	17.2504	PPB	0.00
Spiked Amount	16.700		Recovery	=	103.29%	
64) Toluene-d8 (Surr)	8.08	98	812478	18.3324	PPB	0.00
Spiked Amount	16.700		Recovery	=	109.76%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	284785	17.8052	PPB	0.00
Spiked Amount	16.700		Recovery	=	106.65%	
Target Compounds						
12) Carbon disulfide	3.01	76	25008	0.6142	PPB	91
20) Acetone	3.64	58	1319	2.3100	PPB	# 8


Quantitation Report

Data File : H:\MSI.I\I012609.B\I126914.D
Acq On : 26 Jan 2009 11:59 am
Sample : ASA0086-02 @1X A,REGC
Misc :
MS Integration Params: VOA.P
Quant Time: Jan 27 13:39 19109

Vial: 14
Operator: DY
Inst : MSI
Multiplr: 1.00

Quant Results File: I81104W.RES

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Tue Nov 11 14:35:13 2008
Response via : Initial Calibration

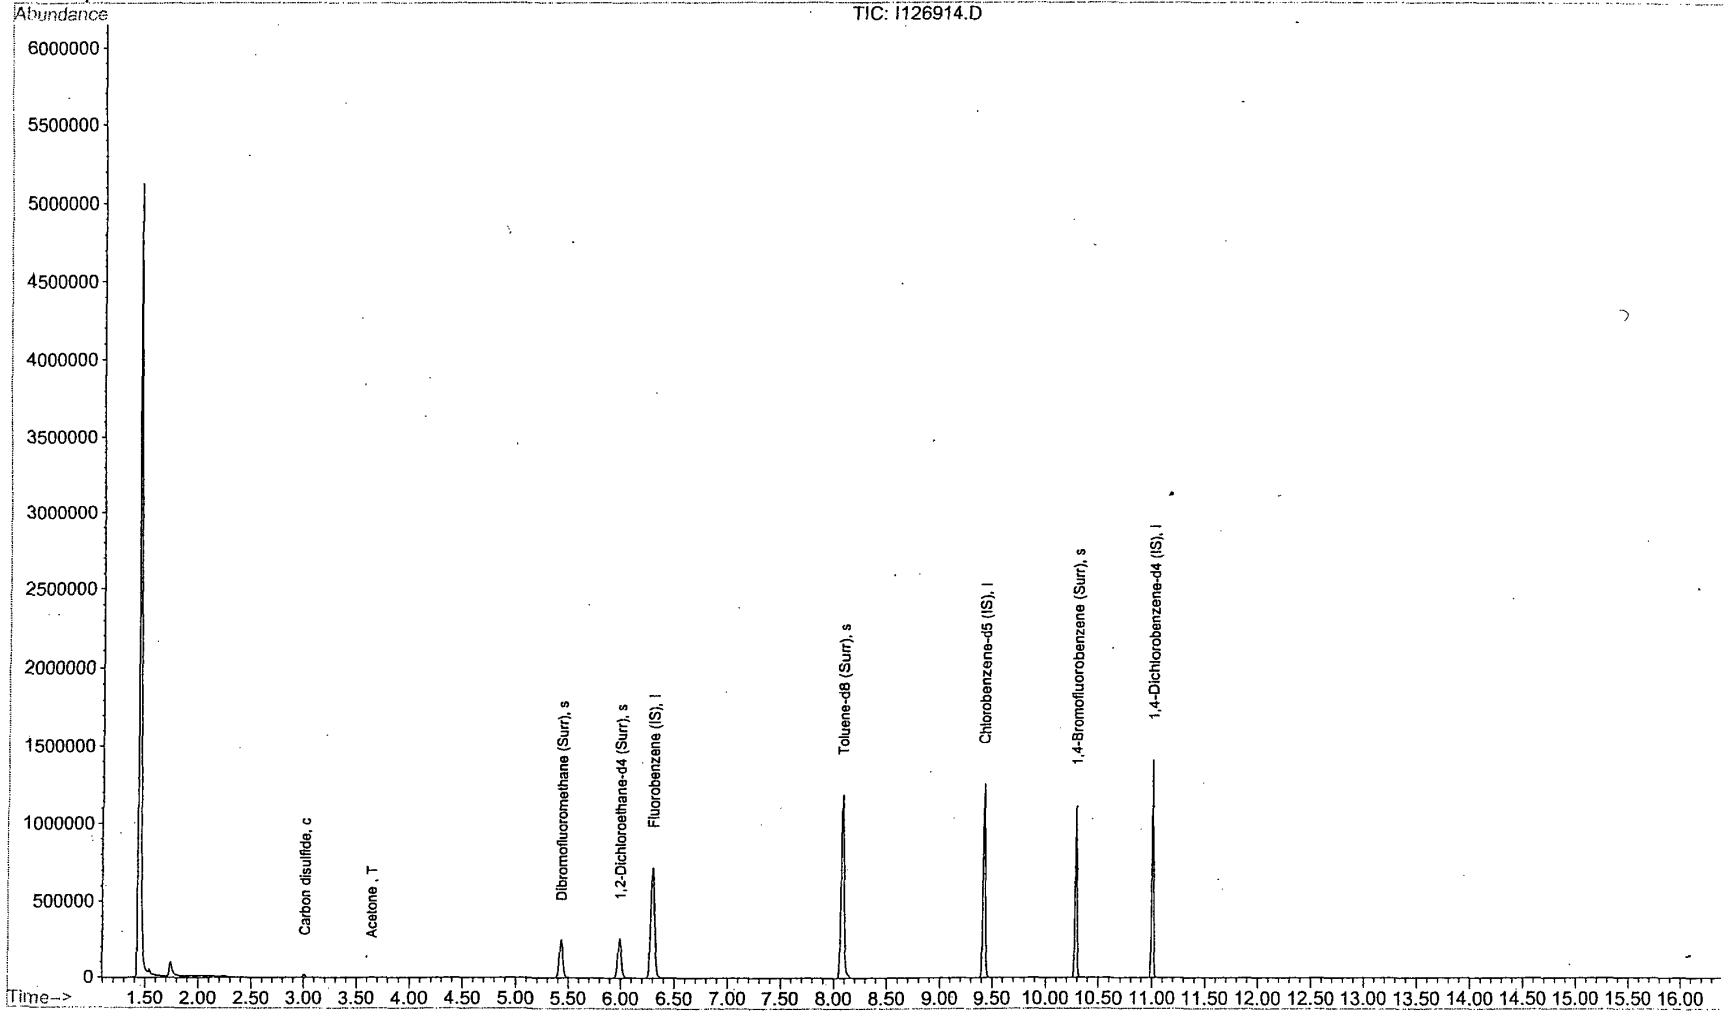

Quantitation Report (QT Reviewed)

61/132

Data File : H:\MSI.I\I012609.B\I126915.D
 Acq On : 26 Jan 2009 12:26 pm
 Sample : ASA0086-03 @1X A,REGC
 Misc :
 MS Integration Params: VOA.P
 Quant Time: Jan 27 13:40 19109

Vial: 15
 Operator: DY
 Inst : MSI
 Multiplr: 1.00

1-29-9 My

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Tue Nov 11 14:49:50 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104w

**Only worked up:
 Target Analytes**

JB

JAN 27 2009

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	754020	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	162460	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.00	152	216689	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	179221	16.2962	PPB	0.00
Spiked Amount	16.700		Recovery	=	97.60%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	102397	16.3192	PPB	0.00
Spiked Amount	16.700		Recovery	=	97.72%	
64) Toluene-d8 (Surr)	8.08	98	783265	18.0924	PPB	0.00
Spiked Amount	16.700		Recovery	=	108.32%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	267128	17.5906	PPB	0.00
Spiked Amount	16.700		Recovery	=	105.33%	
Target Compounds						
6) Ethylene oxide	2.26	44	5213	3.8751	PPB	70
20) Acetone	3.65	58	584	1.0470	PPB #	21


Quantitation Report

Data File : H:\MSI.I\I012609.B\I126915.D
Acq On : 26 Jan 2009 12:26 pm
Sample : ASA0086-03 @1X A,REGC
Misc :
MS Integration Params: VOA.P
Quant Time: Jan 27 13:40 19109

Vial: 15
Operator: DY
Inst : MSI
Multiplr: 1.00

Quant Results File: I81104W.RES

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Tue Nov 11 14:35:13 2008
Response via : Initial Calibration

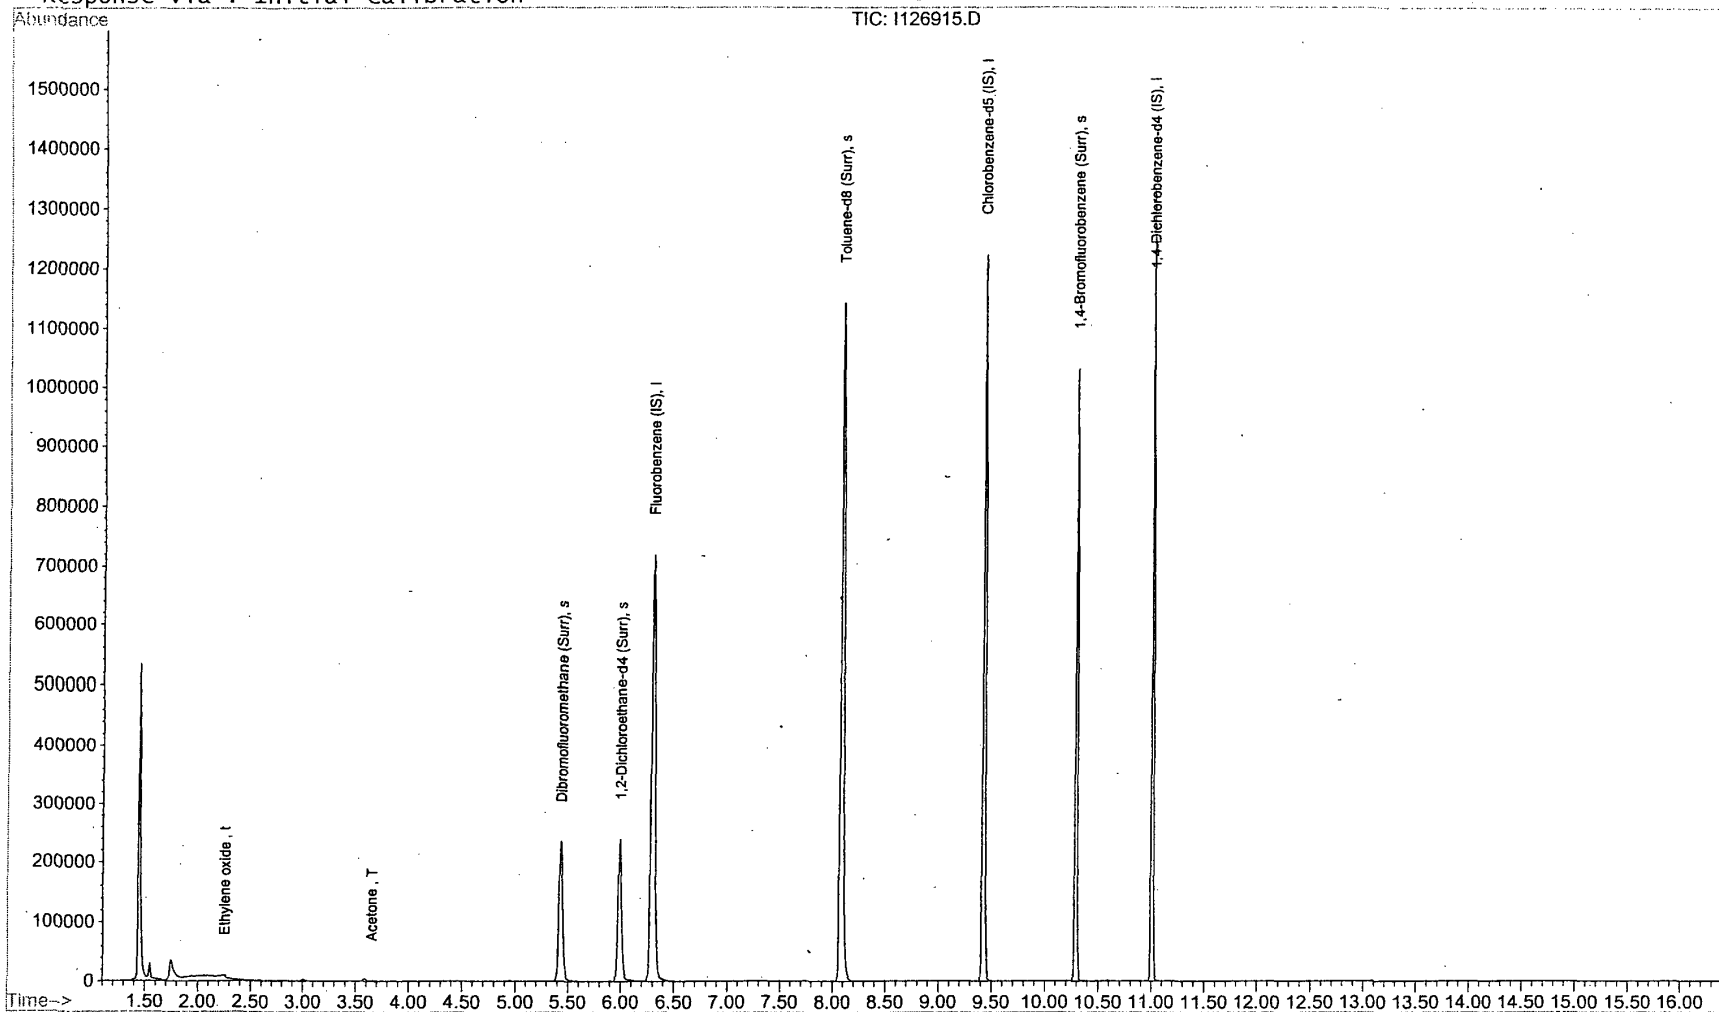

Quantitation Report

(QT Reviewed) 1-263/132

Data File : H:\MSI.I\I012609.B\I126932.D
Acq On : 26 Jan 2009 8:17 pm
Sample : ASA0086-01RE1 @2X A,REGC
Misc : CIS-D
MS Integration Params: VOA.P
Quant Time: Jan 29 14:08 19109

Vial: 32
Operator: DY
Inst : MSI
Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Tue Nov 11 14:49:50 2008
Response via : Initial Calibration
DataAcq Meth : I81104W

Only worked up:
Target Analytes

Cis only-D

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.30	96	637190	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	140199	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.01	152	185347	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	157062	16.8998	PPB	0.00
Spiked Amount	16.700		Recovery	=	101.20%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	94008	17.7293	PPB	0.00
Spiked Amount	16.700		Recovery	=	106.17%	
64) Toluene-d8 (Surr)	8.08	98	678121	18.5357	PPB	0.00
Spiked Amount	16.700		Recovery	=	111.02%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	236973	18.0827	PPB	0.00
Spiked Amount	16.700		Recovery	=	108.26%	
Target Compounds						
32) cis-1,2-Dichloroethene	4.94	96	644137 <i>D</i>	56.9983	PPB	Qvalue 89 ✓


Quantitation Report

Data File : H:\MSI.I\I012609.B\I126932.D
Acq On : 26 Jan 2009 8:17 pm
Sample : ASA0086-01RE1 @2X A,REGC
Misc : CIS-D
MS Integration Params: VOA.P
Quant Time: Jan 29 14:08 19109

Vial: 32
Operator: DY
Inst : MSI
Multiplr: 1.00

Quant Results File: I81104W.RES

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Tue Nov 11 14:35:13 2008
Response via : Initial Calibration

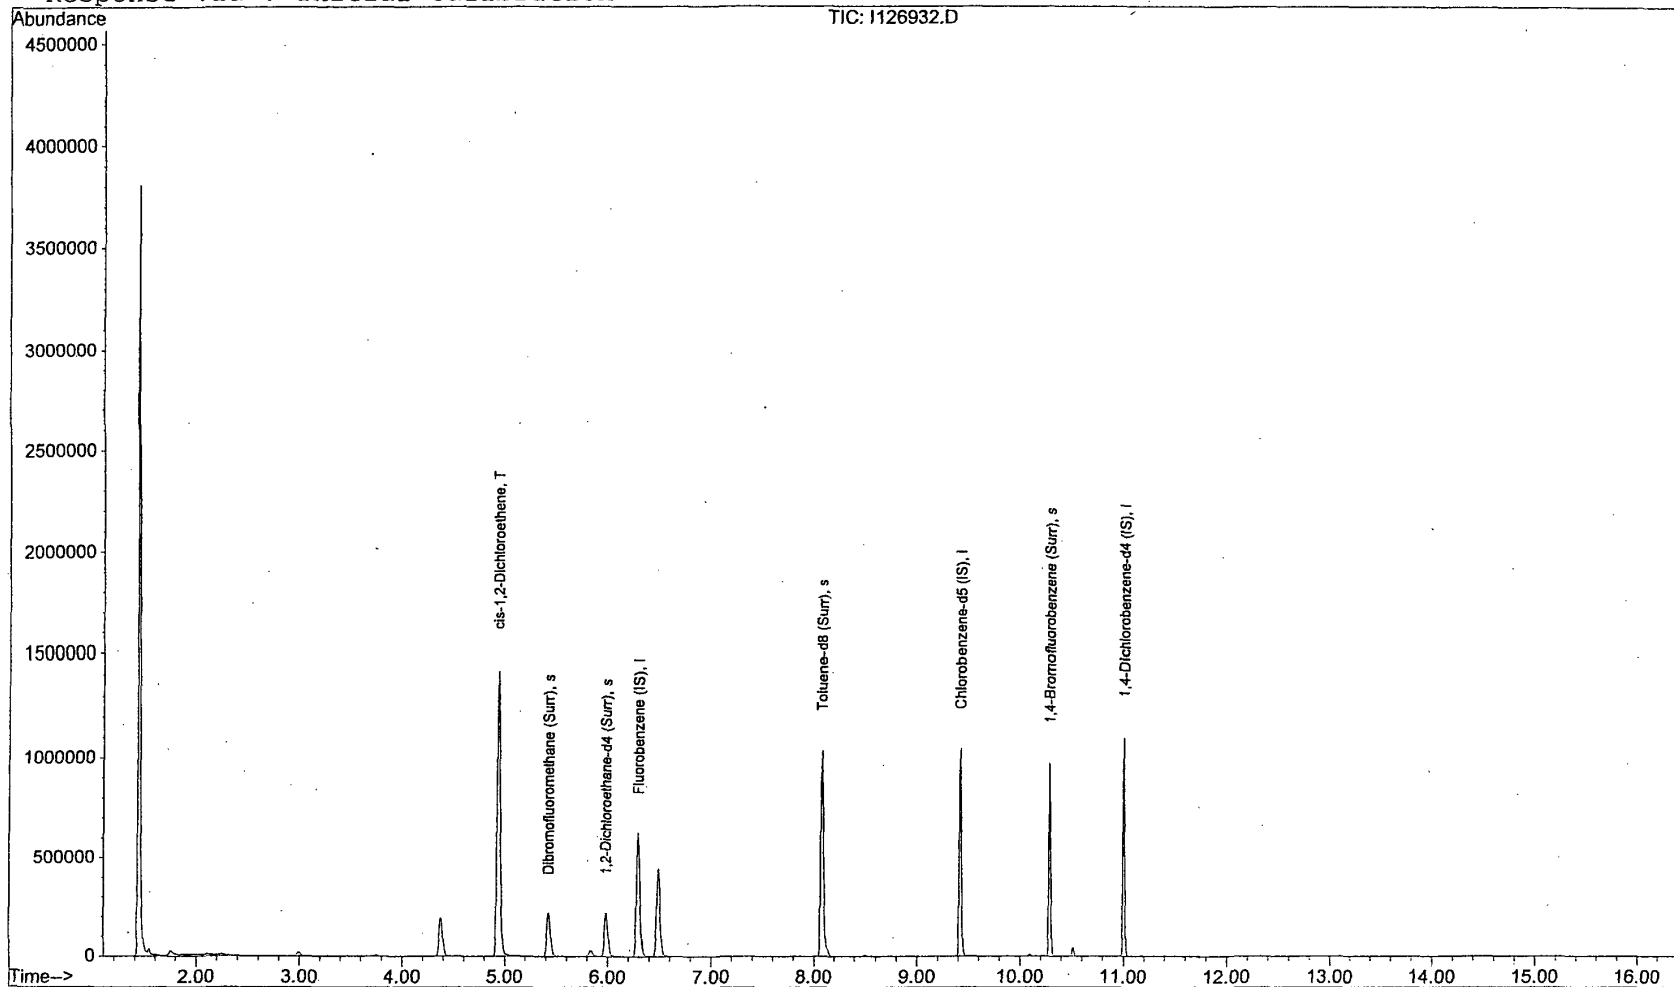

CALIBRATION DATA

TestAmerica Austin

INITIAL CALIBRATION REVIEW FORM

Instrument	MSI
Date Analyzed	11/4/08
Matrix	W

	Analyst check	Peer Reviewer check
Checked to be sure all CCC and SPCC compounds pass criteria.	✓	✓
Checked to be sure all other compounds pass one of the following criteria: RSD<15 for Avg RF, $r^2 \geq 0.990$ for linear, $r^2 \geq 0.990$ for quadratic (minimum 6 points)	NA ✓	✓
Checked to be sure correct levels were used (i.e. none inappropriately skipped).	✓	✓
Checked to be sure that there are at least 5 points for each compound.	✓	✓
Checked to be sure the internal standard concentration is correct (i.e. 16.7 for waters, 50.0 for soils).	✓	✓
Checked to be sure that lowest point matches SOP PQL.	✓	✓
Checked INITIAL CALIBRATION CHECK FORM to be sure all analytes were picked up (i.e. there were no RT values of 0).	✓	✓
Checked INITIAL CALIBRATION CHECK FORM to be sure all isomers have unique RTs (i.e. no analytes at same RT with same primary ion).	✓	✓
Checked that the quant reports for manually-integrated compounds are in the folder and the area counts match those in the method.	NA	N/A
If additional compound(s) calibrated for separately, be sure they use appropriate additional levels (e.g. 1a,2a,3a,4a,5a).	NA	N/A
Included a tune file and sequence file in the ICAL folder.	✓	✓
Included a list of compounds form (shows fit) and plots for those analytes using linear regression (if applicable).	✓	✓
Print ICV form for data folder and instrument. Write NCM for failing ICVs and print NCM for data folder. NCM # 09-0025349	✓	✓
Ran CALEXCEL and saved .xls file in data subdirectory.	✓	✓
Copy Data for Curve Date to Appropriate "DataForCurrentCurve" folder	✓	✓
Verify that (CCV and LCS) macro forms are picking up all analytes	✓	✓
Initial/Date	KA 11/6/08	Boon 11/10/08

****If new analyst or reviewing a new analyst, please take extra time and care.****

Notes:

Clouseau Nonconformance Memo

TestAmerica
THE LEADER IN ENVIRONMENTAL TESTING

NCM #: 09-0025349	Classification: Deficiency
NCM Initiated By: Brian Peterson	Status: QAREVIEW
Date Opened: 11/10/2008	Production Area: MS VOA
Date Closed:	Tests: None
	Lot #'s (Sample #'s): ,
	QC Batches: None.,
Nonconformance: QC data exceeded criteria	
Subcategory: Invalid instrument calibration or calibration verification	

Problem Description / Root Cause

<u>Name</u>	<u>Date</u>	<u>Description</u>
Brian Peterson	11/10/2008	Curve: MSI 11/4/08

The following analytes were not spiked in this curve: 2-Methylhexane, 3-Methylhexane, Heptane and 1,3,5-Trichlorobenzene.

Samples with these target analytes will not be analyzed on this instrument.

The following analyte utilizes quadratic regression fit and will not be reported for South Carolina samples: 1-Chlorohexane.

Corrective Action

<u>Name</u>	<u>Date</u>	<u>Corrective Action</u>
Brian Peterson	11/10/2008	NCM filed, comment "NC" added after appropriate compound name in Enviroquant, and note attached to instrument's monitor.

Client Notification Summary

<u>Client</u>	<u>Project Manager</u>	<u>Notified</u>	<u>Response</u>	<u>How Notified</u>	<u>Note</u>
			<u>Response</u>		<u>Response Note</u>

Quality Assurance Verification

<u>Verified By</u>	<u>Due Date</u>	<u>Status</u>	<u>Notes</u>
			This section not yet completed by QA.

Approval History

<u>Date Approved</u>	<u>Approved By</u>	<u>Position</u>
11/10/2008	Brian Peterson	Group Leader

BMV 11/7/08


Calibration Table Report												
Method: I81104W.M												
Title: EPA Method 8260B/624 Calibration Curve 15mL Water												
Last Calibration: Fri Nov 07 15:27:57 2008												
Calibration Files	0.5	1	2	5	10	20	50	100				
	IB04805.D	IB04806.D	IB04807.D	IB04808.D	IB04809.D	IB04810.D	IB04811.D	IB04812.D				
Compound									Avg	%RSD	LR	QR
										≤15%	≥0.990	≥0.990
Fluorobenzene (IS)	ISTD											
Dichlorodifluoromethane	0.441	0.388	0.347	0.374	0.368	0.362	0.353	0.320	0.369	9.558		
Chloromethane (SPCC)	0.392	0.363	0.333	0.369	0.347	0.358	0.366	0.367	0.362	4.768		
Vinyl chloride (CCC)	0.446	0.408	0.355	0.386	0.384	0.388	0.391	0.372	0.391	6.805		
Bromomethane	✓	0.252	0.207	0.192	0.174	0.180	0.201	0.222	0.204	13.025		
Ethylene oxide	✓	0.034	0.030	0.030	0.028	0.027			0.030	9.288		
Chloroethane	0.309	0.292	0.262	0.264	0.264	0.263	0.255	0.205	0.264	11.403		
Trichlorofluoromethane	0.494	0.430	0.384	0.405	0.397	0.392	0.387	0.354	0.405	10.221		
Ethyl ether	0.227	0.211	0.202	0.203	0.206	0.208	0.205	0.199	0.208	4.205		
Ethanol	✓	0.001	0.001	0.001	0.001	0.001	0.002	0.001	0.001	6.316		
1,1-Dichloroethene (CCC)	0.286	0.256	0.226	0.241	0.242	0.248	0.253	0.250	0.250	6.897		
Carbon disulfide	0.964	0.846	0.797	0.843	0.871	0.896	0.924	0.906	0.881	5.986		
1,1,2-Trichlorotrifluoroethane	0.289	0.261	0.224	0.237	0.233	0.234	0.234	0.219	0.242	9.442		
Propylene oxide	0.029	0.029	0.027	0.029	0.031	0.031	0.031	0.029	0.030	4.312		
Iodomethane	✓	0.139	0.173	0.261	0.338	0.375	0.388	0.387	0.294	35.546	1.000	
Bromoethane	0.222	0.205	0.197	0.194	0.200	0.202	0.202	0.205	0.203	4.101		
Acrolein	0.013	0.013	0.013	0.014	0.015	0.015	0.016	0.016	0.014	8.790		
3-Chloropropene	0.535	0.489	0.483	0.503	0.516	0.523	0.517	0.496	0.508	3.539		
Methylene chloride	0.329	0.301	0.275	0.276	0.279	0.278	0.277	0.273	0.286	6.845		
Acetone	✓	0.011	0.012	0.011	0.013	0.013	0.013	0.013	0.012	6.517		
trans-1,2-Dichloroethene	0.320	0.277	0.264	0.272	0.275	0.278	0.280	0.283	0.281	5.905		
Methyl acetate	0.021	0.021	0.020	0.022	0.022	0.022	0.022	0.022	0.021	4.343		
Hexane	0.107	0.094	0.086	0.092	0.093	0.094	0.095	0.088	0.094	6.806		
Methyl tert-butyl ether (MTBE)	0.606	0.596	0.558	0.572	0.590	0.590	0.589	0.569	0.584	2.743		
tert-Butyl alcohol	0.010	0.011	0.011	0.010	0.012	0.012	0.013	0.012	0.011	8.127		
Acetonitrile	0.012	0.010	0.010	0.010	0.010	0.010	0.010	0.009	0.010	6.460		
Isopropyl ether	1.085	1.034	0.993	1.021	1.051	1.059	1.034	0.979	1.032	3.333		
2-Chloro-1,3-butadiene	0.214	0.194	0.185	0.209	0.222	0.233	0.238	0.237	0.217	9.134		

Calibration Files	0.5	1	2	5	10	20	50	100				
	IB04805.D	IB04806.D	IB04807.D	IB04808.D	IB04809.D	IB04810.D	IB04811.D	IB04812.D				
Compound									Avg	%RSD	LR	QR
										≤15%	≥0.990	≥0.990
1,1-Dichloroethane (SPCC)	0.616	0.567	0.534	0.536	0.546	0.546	0.536	0.523	0.551	5.316		
Acrylonitrile	0.054	0.053	0.050	0.052	0.054	0.053	0.053	0.052	0.053	2.661		
Vinyl acetate	0.302	0.291	0.304	0.326	0.355	0.365	0.368	0.354	0.333	9.333		
cis-1,2-Dichloroethene	0.323	0.291	0.283	0.284	0.293	0.295	0.300	0.301	0.296	4.186		
2,2-Dichloropropane	0.443	0.423	0.386	0.406	0.413	0.419	0.413	0.401	0.413	4.074		
Cyclohexane	0.594	0.521	0.472	0.515	0.513	0.509	0.509	0.470	0.513	7.458		
Bromochloromethane	0.147	0.140	0.130	0.131	0.136	0.140	0.141	0.144	0.139	4.251		
2-Methylhexane (NC)												
Chloroform (CCC)	0.524	0.488	0.461	0.467	0.469	0.468	0.466	0.460	0.475	4.498		
Carbon tetrachloride	0.353	0.322	0.290	0.319	0.326	0.326	0.323	0.314	0.322	5.390		
3-Methylhexane (NC)												
Ethyl acetate	0.134	0.130	0.127	0.131	0.139	0.138	0.136	0.128	0.133	3.447		
Tetrahydrofuran			0.017	0.017	0.020	0.020	0.021	0.020	0.019	8.500		
Dibromofluoromethane (Surr)	0.253	0.242	0.228	0.234	0.244	0.246	0.249	0.251	0.244	3.584		
1,1,1-Trichloroethane	0.438	0.401	0.369	0.395	0.396	0.396	0.399	0.388	0.398	4.782		
1,1-Dichloropropene	0.413	0.376	0.351	0.377	0.387	0.387	0.388	0.378	0.382	4.573		
2-Butanone (MEK)	0.071	0.070	0.052	0.054	0.058	0.060	0.061	0.059	0.060	11.154		
Benzene	1.323	1.211	1.149	1.168	1.194	1.208	1.201	1.180	1.204	4.360		
Heptane (NC)												
Propanenitrile	0.018	0.019	0.019	0.020	0.020	0.020	0.021	0.020	0.020	4.419		
Methacrylonitrile	0.061	0.058	0.058	0.063	0.067	0.067	0.068	0.066	0.063	6.629		
1,2-Dichloroethane-d4 (Surr)	0.167	0.156	0.140	0.133	0.133	0.132	0.127	0.124	0.139	10.694		
1,2-Dichloroethane	0.334	0.306	0.291	0.281	0.291	0.282	0.275	0.265	0.291	7.306		
Isobutyl alcohol	0.004	0.004	0.004	0.005	0.005	0.006	0.006	0.006	0.005	17.006	0.999	
Methylcyclohexane	0.412	0.372	0.331	0.356	0.358	0.358	0.366	0.343	0.362	6.641		
Trichloroethene	0.317	0.276	0.264	0.264	0.269	0.274	0.281	0.288	0.279	6.240		
Dibromomethane	0.112	0.102	0.098	0.100	0.106	0.107	0.107	0.107	0.105	4.344		
n-Butanol	0.002	0.002	0.002	0.002	0.003	0.004	0.004	0.004	0.003	29.253	0.999	
1,2-Dichloropropane (CCC)	0.311	0.280	0.267	0.271	0.282	0.282	0.281	0.279	0.282	4.609		
Bromodichloromethane	0.334	0.306	0.297	0.313	0.331	0.331	0.335	0.338	0.323	4.821		
1,4-Dioxane	0.001	0.001	0.001	0.001	0.001	0.001	0.001	0.001	0.001	12.800		
Methyl methacrylate	0.079	0.072	0.080	0.089	0.102	0.109	0.116	0.116	0.095	18.534	1.000	
1-Bromo-2-chloroethane	0.320	0.304	0.283	0.281	0.297	0.299	0.300	0.297	0.298	4.061		
cis-1,3-Dichloropropene	0.373	0.359	0.362	0.381	0.418	0.428	0.434	0.431	0.398	8.196		

Calibration Files	0.5	1	2	5	10	20	50	100				
	IB04805.D	IB04806.D	IB04807.D	IB04808.D	IB04809.D	IB04810.D	IB04811.D	IB04812.D				
Compound									Avg	%RSD	LR	QR
										≤15%	≥0.990	≥0.990
2-Chloroethyl vinyl ether	✓	✓	0.070	0.076	0.087	0.090	0.092	0.088	0.084	10.583		
Toluene-d8 (Surr)	0.985	0.936	0.892	0.920	0.964	0.983	0.997	0.993	0.959	4.022		
Chlorobenzene-d5 (IS)	ISTD											
Toluene (CCC)	6.128	5.837	5.563	5.599	5.668	5.672	5.395	5.240	5.638	4.769		
Epichlorohydrin	0.056	0.051	0.054	0.057	0.061	0.062	0.061	0.057	0.057	6.453		
2-Nitropropane	✓	✓	✓	0.114	0.130	0.146	0.157	0.161	0.142	13.697		
Tetrachloroethene	1.107	0.964	0.865	0.909	0.916	0.907	0.900	0.896	0.933	8.078		
4-Methyl-2-pentanone (MIBK)	0.496	0.501	0.529	0.559	0.612	0.639	0.626	0.586	0.569	9.857		
trans-1,3-Dichloropropene	1.335	1.306	1.365	1.449	1.575	1.594	1.518	1.478	1.452	7.483		
1,1,2-Trichloroethane	0.789	0.787	0.775	0.774	0.787	0.771	0.738	0.728	0.769	2.982		
4-Methyl-2-pentanol (MIBC)	✓	0.066	0.073	0.080	0.098	0.110	0.133	0.132	0.099	27.716	0.999	
Ethyl methacrylate	✓	0.683	0.770	0.862	1.024	1.087	1.096	1.070	0.942	17.932	1.000	
Dibromochloromethane	0.790	0.763	0.755	0.810	0.867	0.898	0.875	0.874	0.829	6.777		
1,3-Dichloropropane	1.792	1.628	1.559	1.544	1.575	1.540	1.448	1.406	1.562	7.501		
1,2-Dibromoethane (EDB)	0.717	0.675	0.652	0.670	0.699	0.688	0.677	0.658	0.680	3.154		
2-Hexanone	✓	0.294	0.341	0.373	0.379	0.398	0.384	0.658	0.349	13.380		
Chlorobenzene (SPCC)	4.063	3.634	3.357	3.337	3.351	3.370	3.354	3.328	3.474	7.432		
1-Chlorohexane	2.543	1.872	1.475	1.414	1.341	1.307	1.207	1.102	1.533	30.526		1.000
Ethylbenzene (CCC)	2.240	1.980	1.834	1.895	1.960	1.971	1.938	1.943	1.970	6.034		
1,1,1,2-Tetrachloroethane	1.089	1.069	1.005	1.036	1.083	1.086	1.068	1.071	1.063	2.699		
m&p-Xylene	2.617	2.431	2.299	2.369	2.462	2.468	2.475	2.408	2.441	3.794		
o-Xylene	2.318	2.207	2.099	2.196	2.328	2.333	2.311	2.303	2.262	3.753		
Bromoform (SPCC)	0.328	0.320	0.325	0.350	0.393	0.405	0.419	0.425	0.371	12.053		
Styrene	2.870	2.782	2.894	3.347	3.660	3.759	3.756	3.734	3.350	13.043		
Isopropylbenzene	5.543	5.274	5.038	5.347	5.450	5.485	5.328	5.180	5.331	3.132		
Bromobenzene	1.178	1.092	1.083	1.100	1.143	1.139	1.153	1.185	1.134	3.412		
n-Propylbenzene	1.477	1.421	1.412	1.500	1.554	1.552	1.578	1.593	1.511	4.607		
1,1,2,2-Tetrachloroethane (SPCC)	0.835	0.823	0.781	0.780	0.801	0.795	0.788	0.773	0.797	2.739		
1,4-Bromofluorobenzene (Surr)	1.702	1.601	1.511	1.523	1.563	1.576	1.516	1.497	1.561	4.314		
1,4-Dichlorobenzene-d4 (IS)	ISTD											
2-Chlorotoluene	1.043	0.978	0.910	0.941	0.965	0.968	0.983	0.973	0.970	3.922		
Cyclohexanone	✓	✓	0.009	0.009	0.010	0.009	0.011	0.010	0.010	7.259		
1,2,3-Trichloropropane	0.222	0.211	0.202	0.197	0.198	0.194	0.193	0.185	0.200	5.817		
trans-1,4-Dichloro-2-butene	✓	0.116	0.125	0.137	0.157	0.163	0.173	0.165	0.148	14.834		


Calibration Files	0.5	1	2	5	10	20	50	100				
	IB04805.D	IB04806.D	IB04807.D	IB04808.D	IB04809.D	IB04810.D	IB04811.D	IB04812.D				
Compound									Avg	%RSD	LR	QR
										≤15%	≥0.990	≥0.990
3-Ethyltoluene	4.196	4.007	3.905	4.103	4.262	4.254	4.264	4.038	4.129	3.304		
4-Chlorotoluene	1.027	0.945	0.911	0.931	0.965	0.977	0.975	0.962	0.962	3.610		
1,3,5-Trimethylbenzene	3.600	3.445	3.300	3.467	3.562	3.592	3.539	3.390	3.487	3.041		
2-Ethyltoluene	4.365	4.202	4.032	4.131	4.289	4.270	4.199	3.991	4.185	3.060		
tert-Butylbenzene	2.107	1.974	1.854	1.910	1.926	1.914	1.859	1.765	1.914	5.217		
Pentachloroethane	0.428	0.413	0.442	0.459	0.503	0.534	0.551	0.567	0.487	12.216		
1,2,4-Trimethylbenzene	3.486	3.476	3.340	3.441	3.594	3.616	3.575	3.406	3.492	2.783		
sec-Butylbenzene	4.697	4.321	4.041	4.179	4.281	4.286	4.264	4.005	4.259	4.985		
p-Isopropyltoluene	3.688	3.555	3.407	3.595	3.740	3.763	3.772	3.599	3.640	3.449		
1,3-Dichlorobenzene	1.938	1.757	1.656	1.636	1.690	1.710	1.724	1.712	1.728	5.396		
1,4-Dichlorobenzene	2.125	1.908	1.769	1.726	1.775	1.761	1.799	1.770	1.829	7.153		
Benzyl chloride	✓	✓	0.102	0.139	0.169	0.204	0.242	0.261	0.186	32.922	0.999	
n-Butylbenzene	0.862	0.784	0.734	0.818	0.871	0.893	0.917	0.917	0.850	7.745		
1,2-Dichlorobenzene	1.568	1.459	1.355	1.371	1.434	1.445	1.436	1.428	1.437	4.459		
1,3,5-Trichlorobenzene (NC)												
1,2-Dibromo-3-chloropropane (DBCP)	✓	0.049	0.052	0.059	0.066	0.073	0.086	0.084	0.067	21.793	0.999	
Hexachlorobutadiene	0.486	0.467	0.411	0.413	0.417	0.421	0.438	0.435	0.436	6.217		
1,2,4-Trichlorobenzene	0.763	0.758	0.694	0.732	0.780	0.801	0.812	0.799	0.767	5.190		
Naphthalene	0.898	0.954	0.984	1.070	1.208	1.273	1.305	1.237	1.116	14.253		
1,2,3-Trichlorobenzene	0.552	0.551	0.526	0.522	0.552	0.554	0.559	0.544	0.545	2.483		

Fri Nov 07 15:34:57 2008

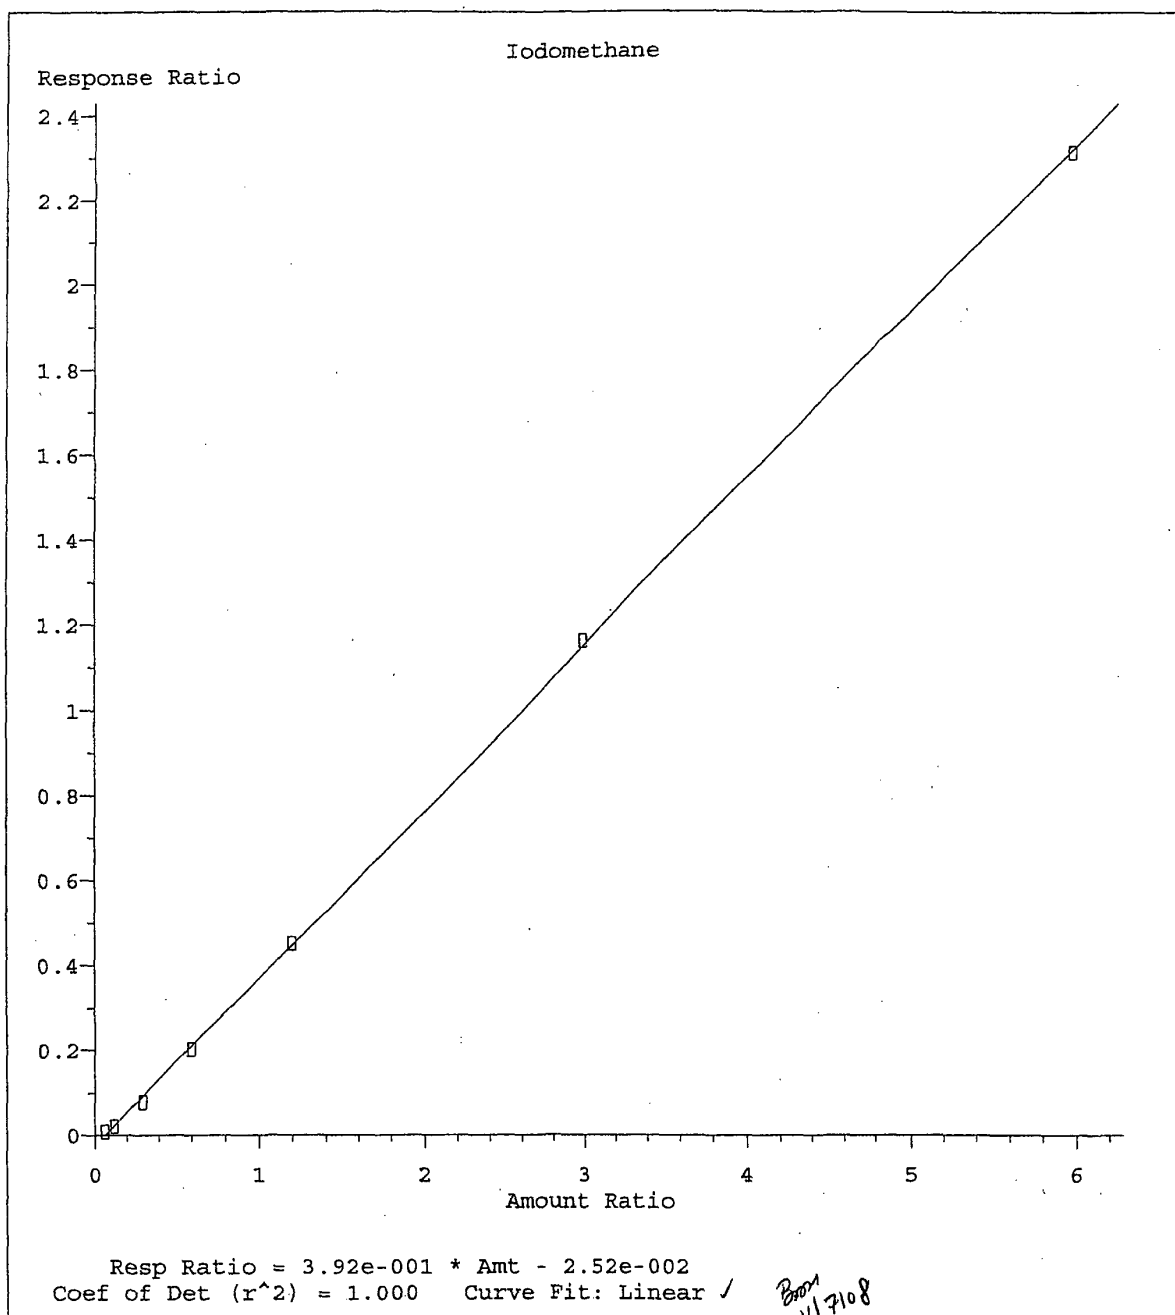


Method Name: H:\MSI.I\METHODS\I81104W.M
Calibration Table Last Updated: Fri Nov 07 15:04:06 2008

RA 11/5/08

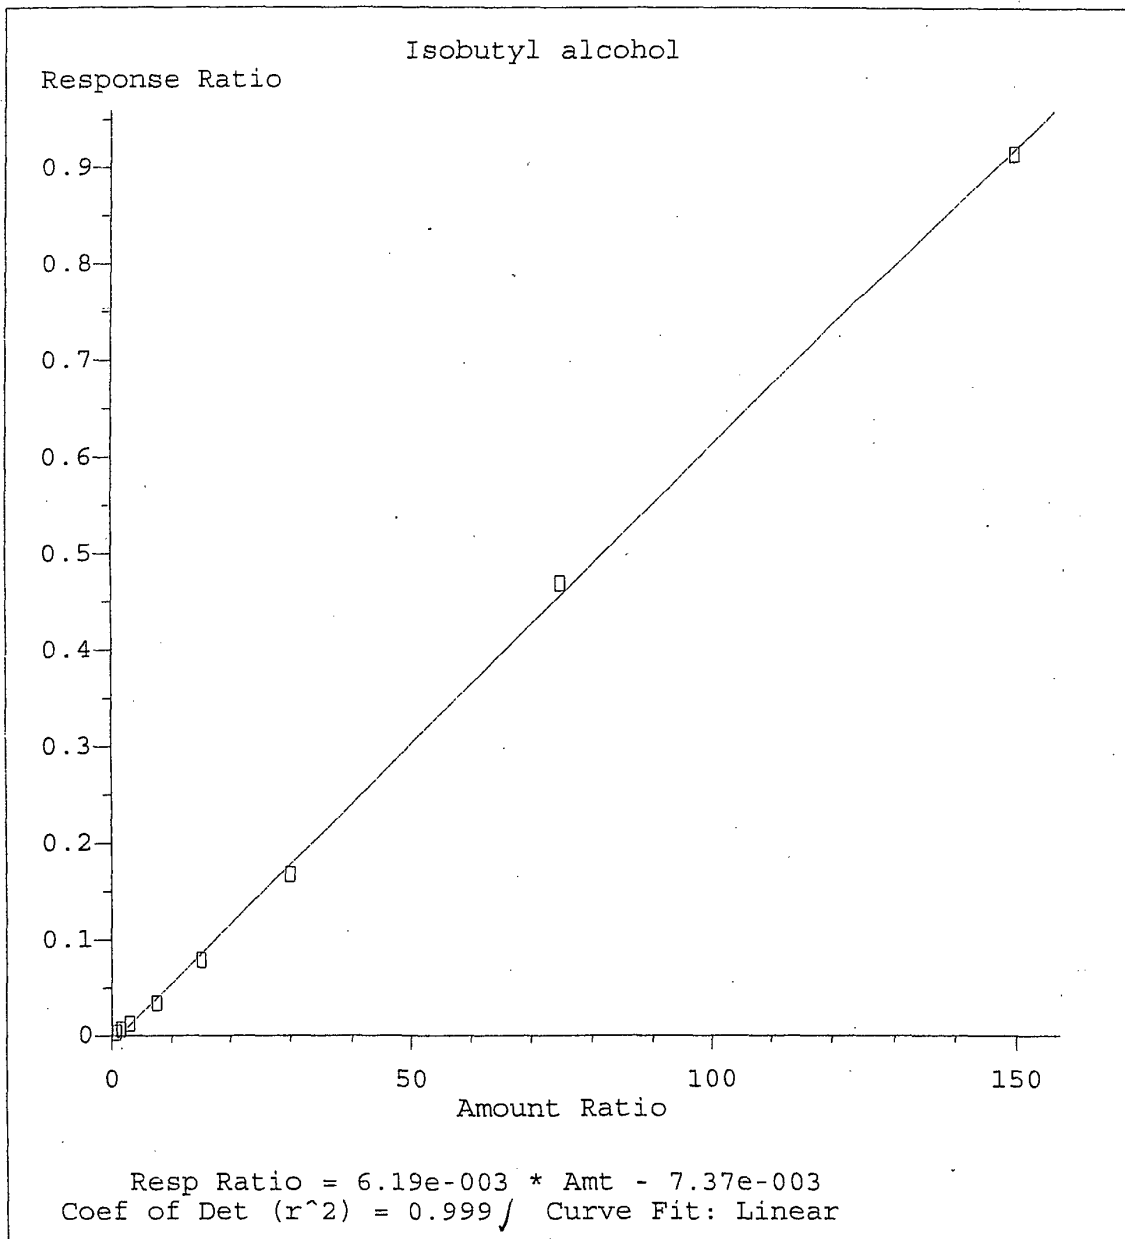


Method Name: H:\MSI.I\METHODS\I81104W.M
Calibration Table Last Updated: Wed Nov 05 10:33:32 2008

.PA 11/5/08

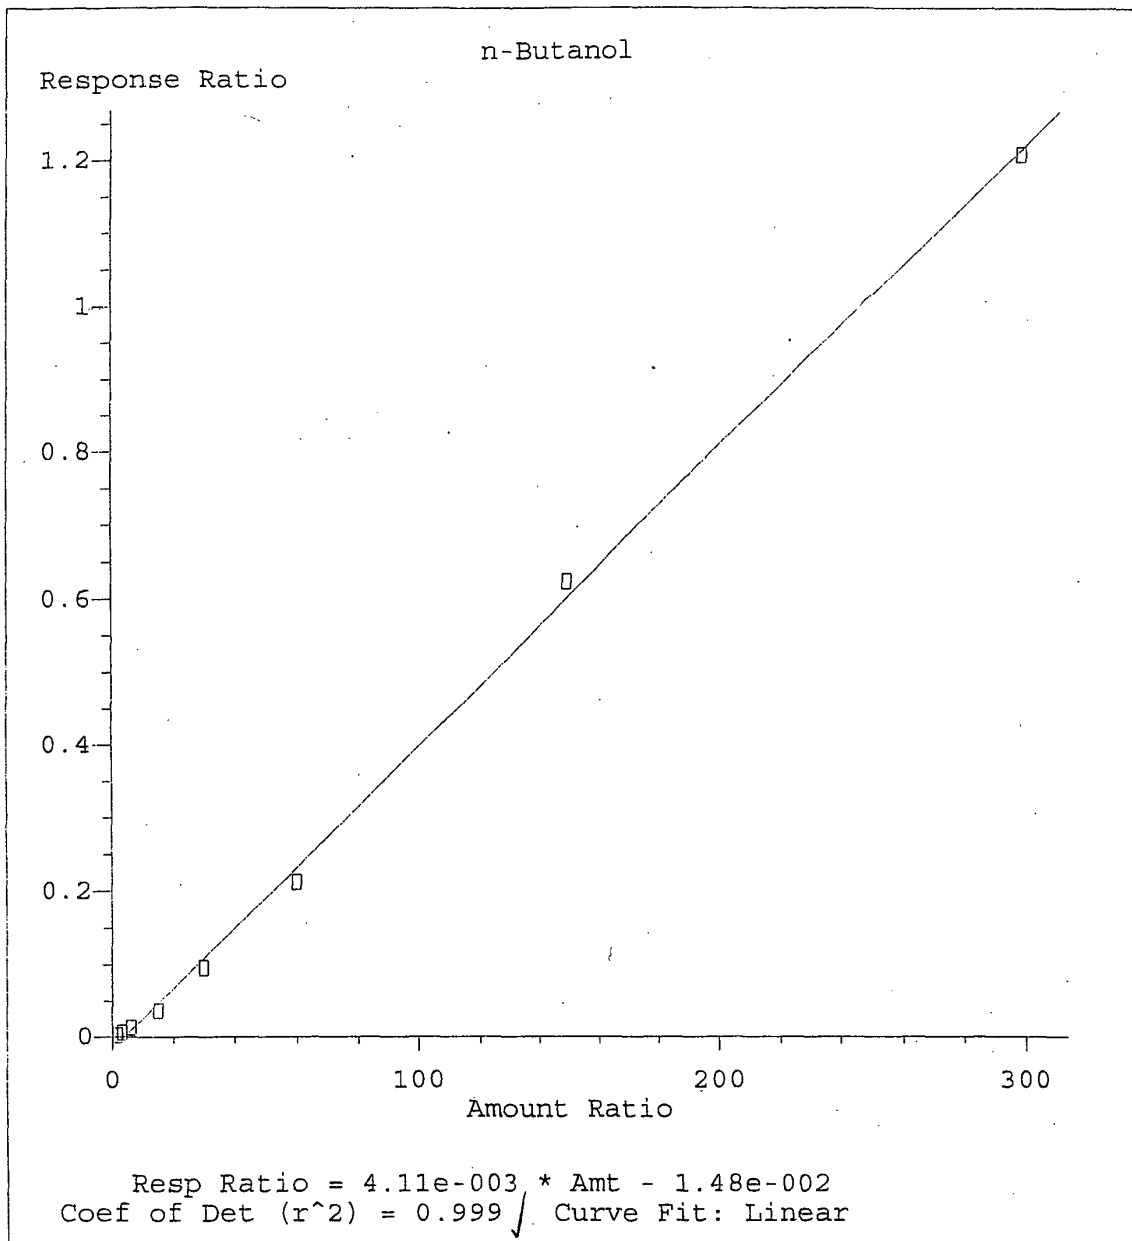


Method Name: H:\MSI.I\METHODS\I81104W.M
Calibration Table Last Updated: Wed Nov 05 10:35:55 2008

11/5/08

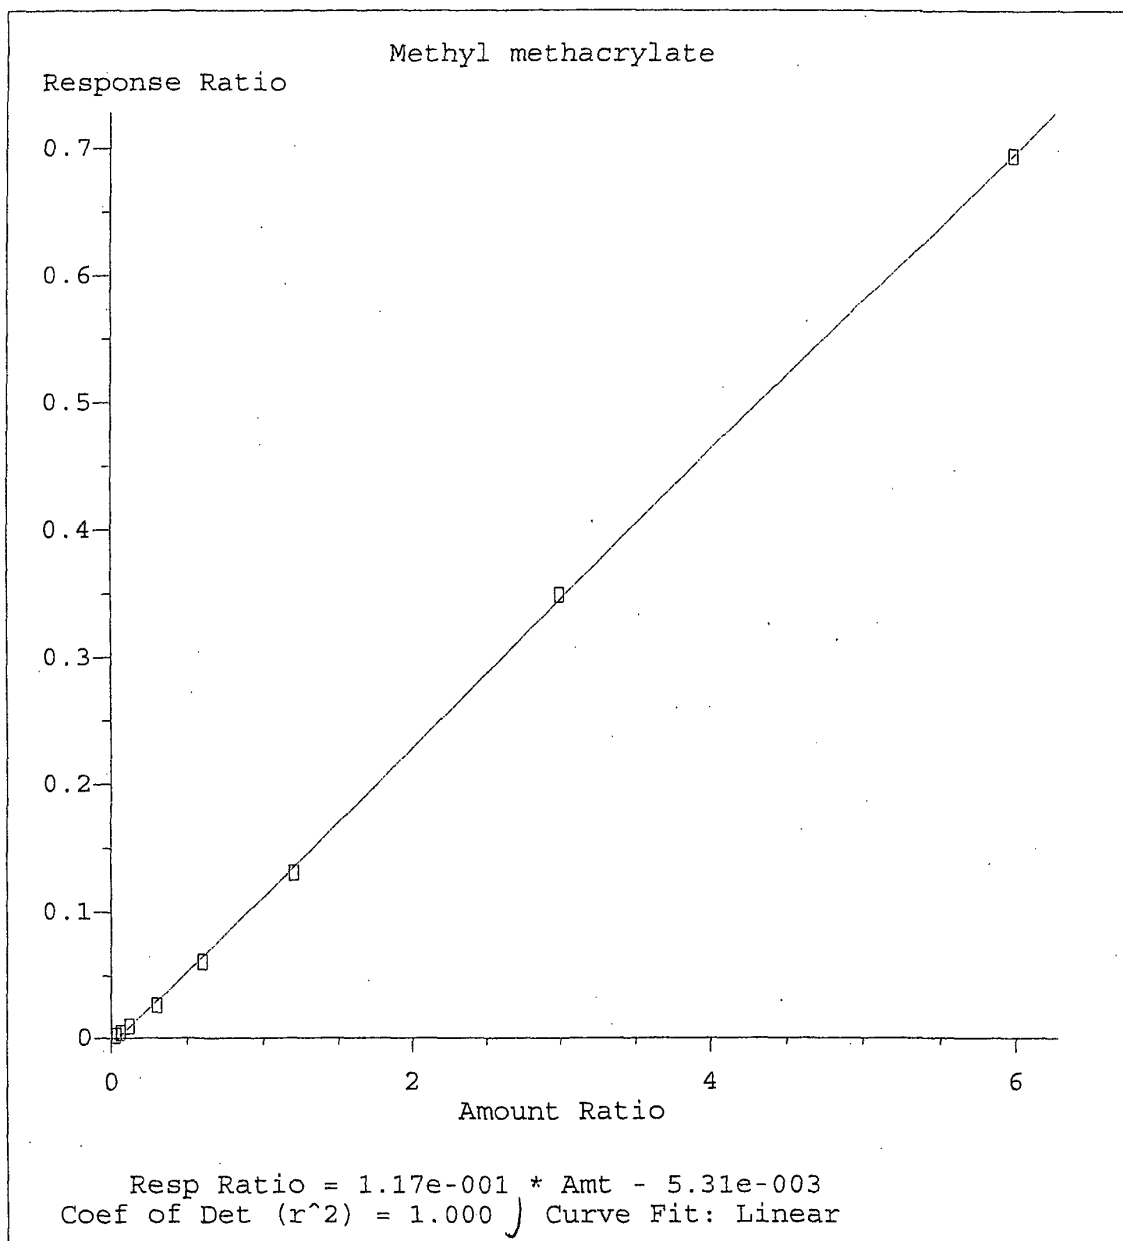


Method Name: H:\MSI.I\METHODS\I81104W.M
Calibration Table Last Updated: Wed Nov 05 10:41:25 2008

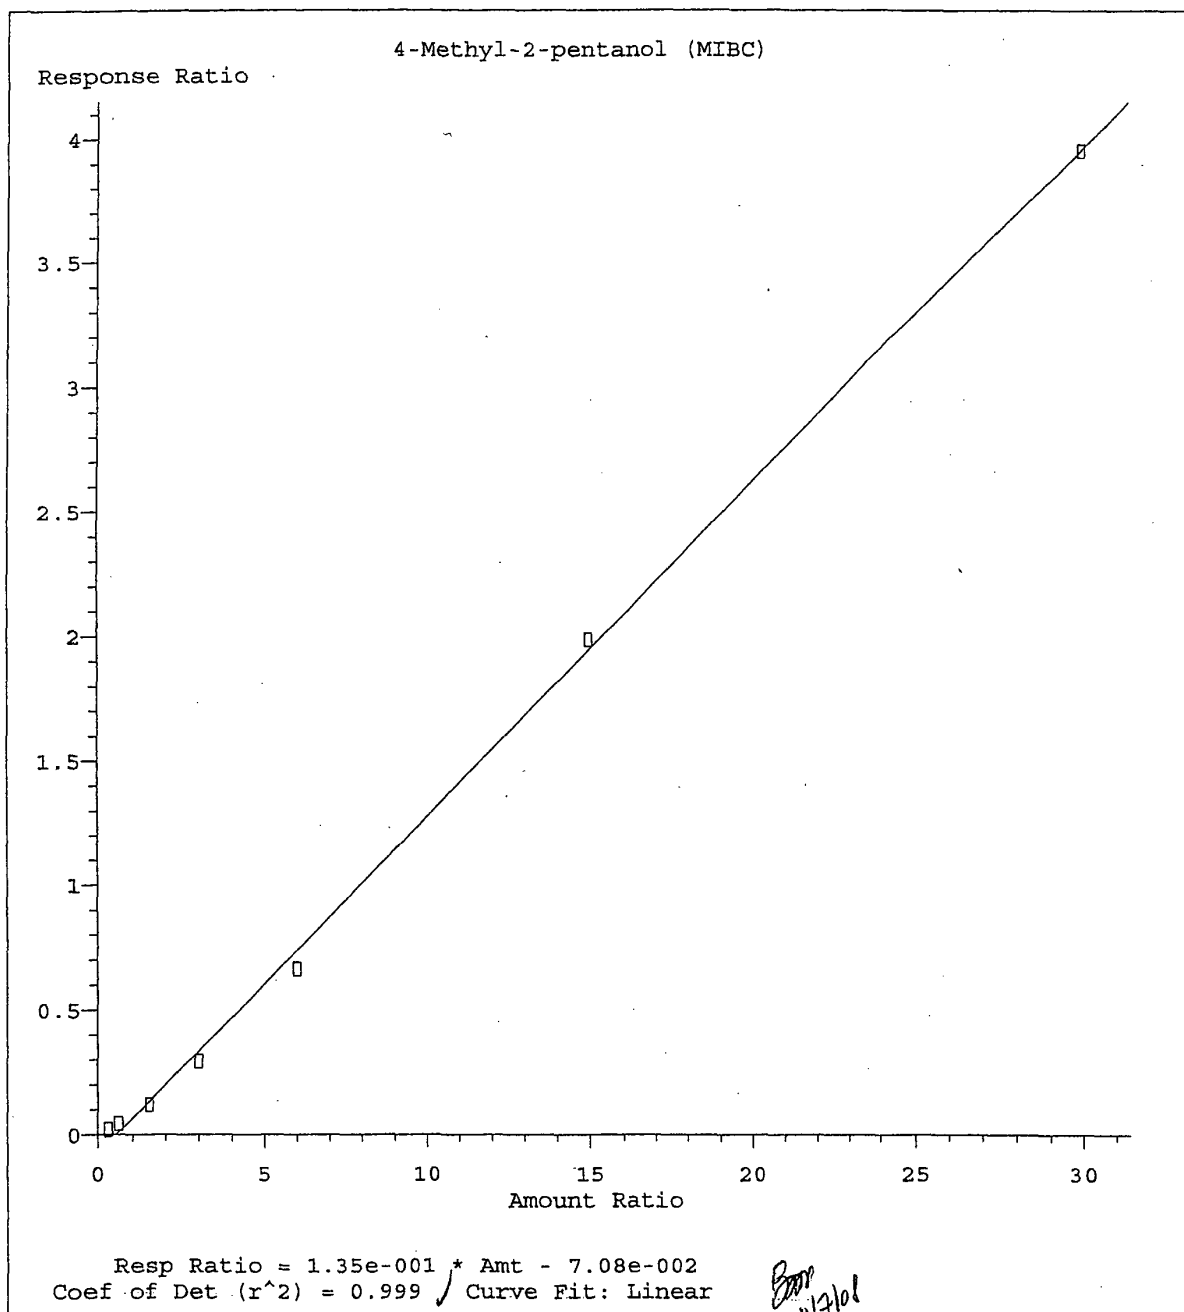


Method Name: H:\MSI.I\METHODS\I81104W.M
Calibration Table Last Updated: Fri Nov 07 14:54:09 2008


KA 11/5/08

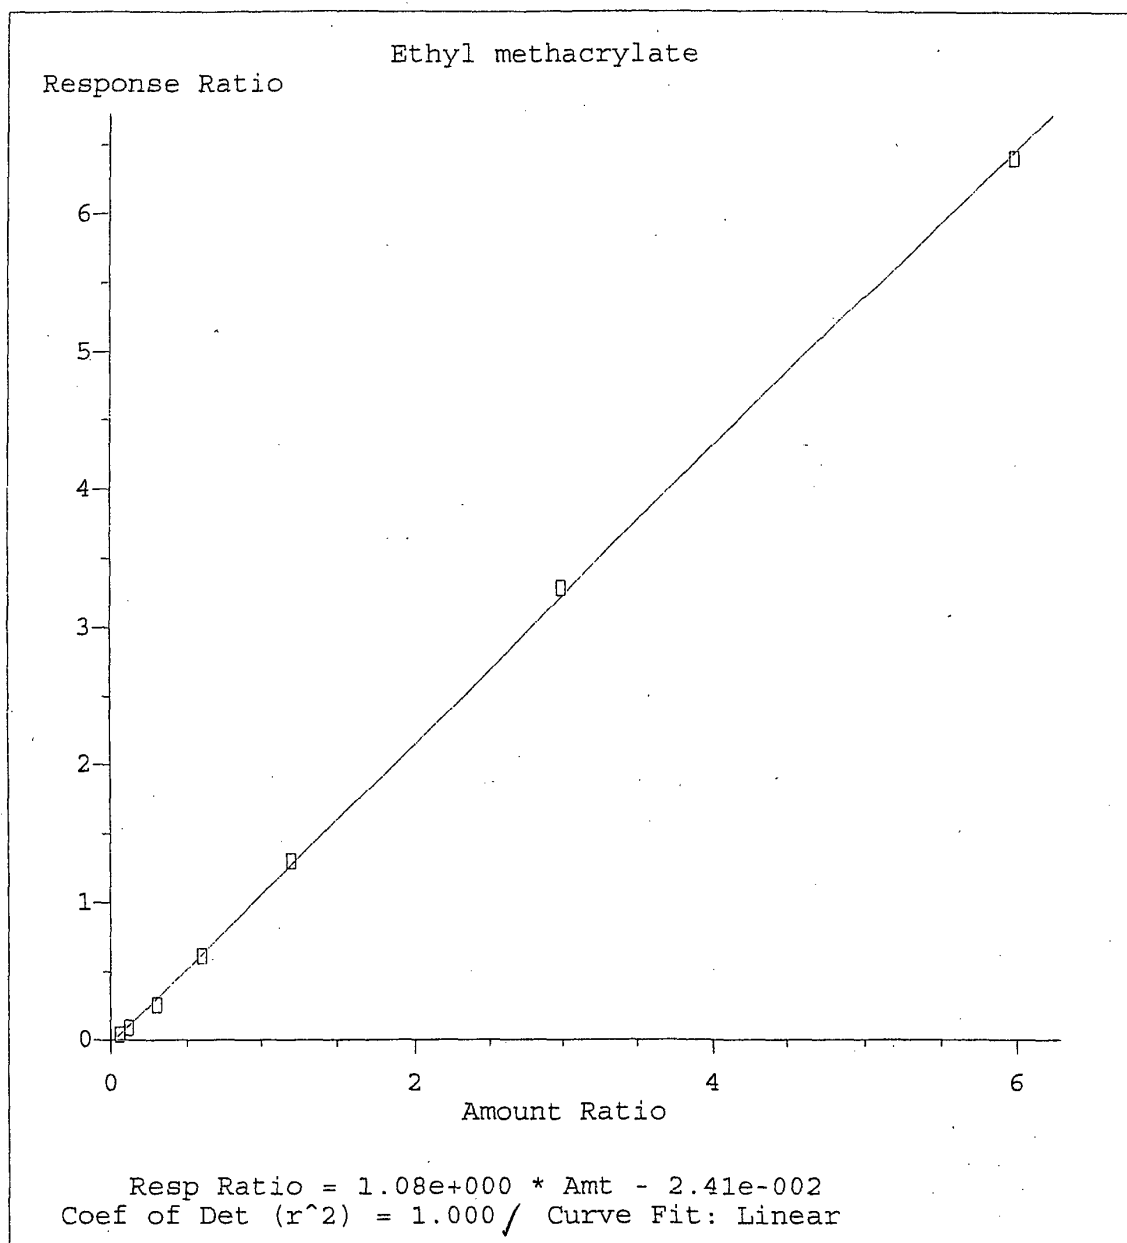


Method Name: H:\MSI.I\METHODS\I81104W.M
Calibration Table Last Updated: Wed Nov 05 10:52:49 2008

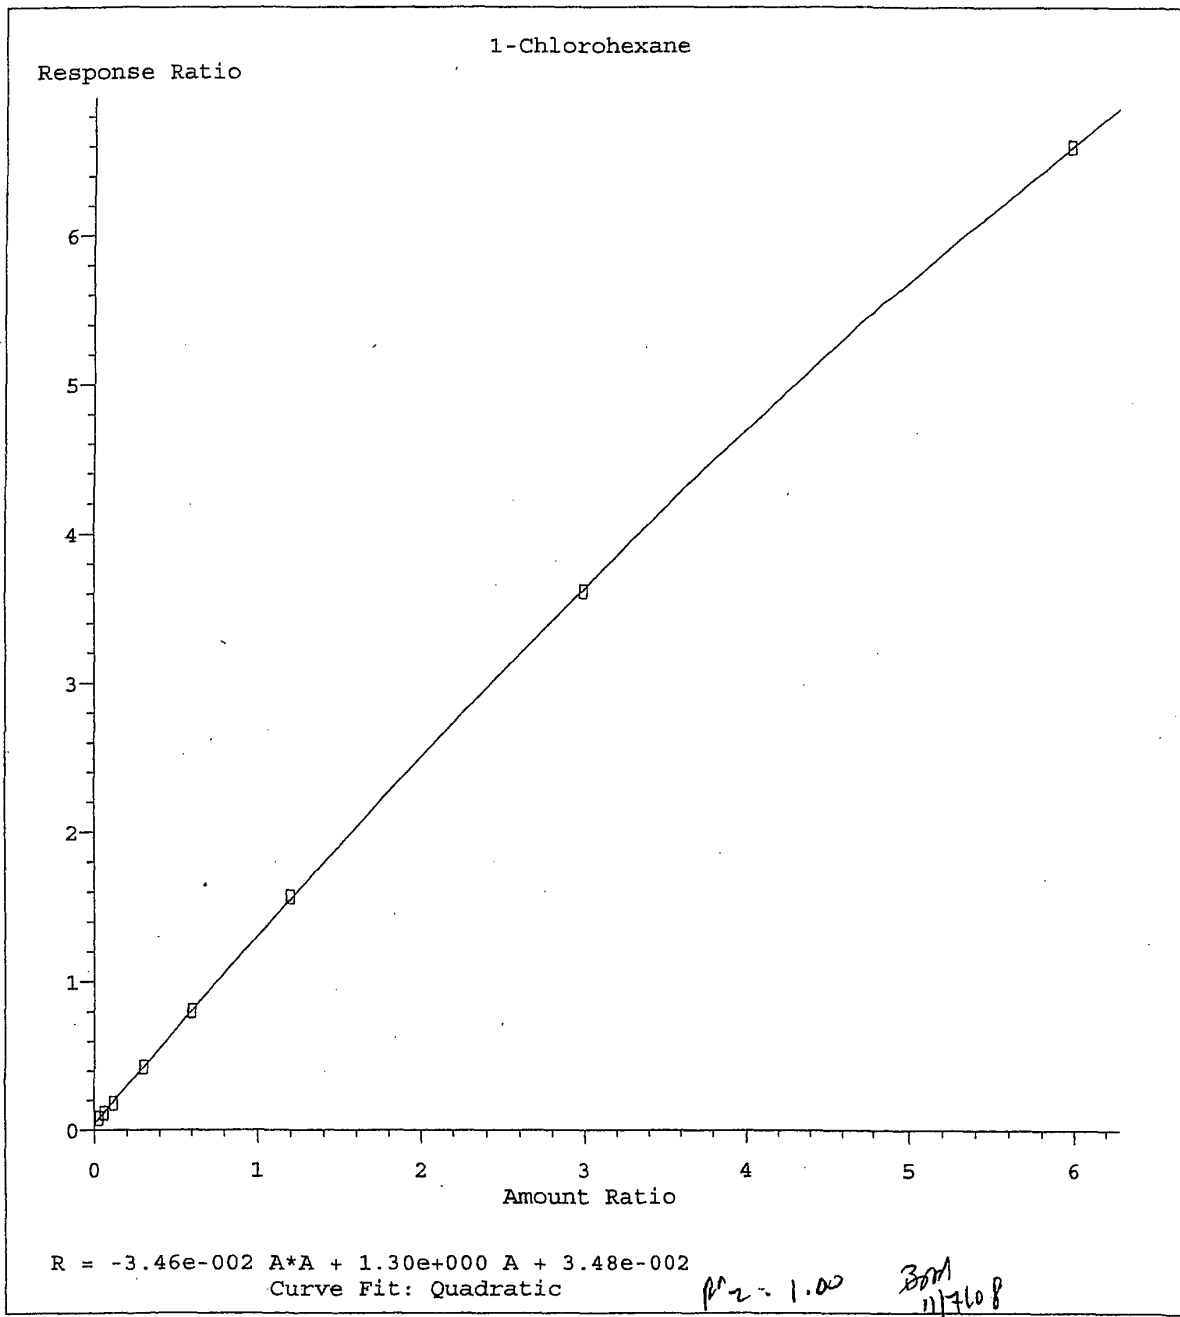

Method Name: H:\MSI.I\METHODS\I81104W.M
Calibration Table Last Updated: Fri Nov 07 15:27:57 2008

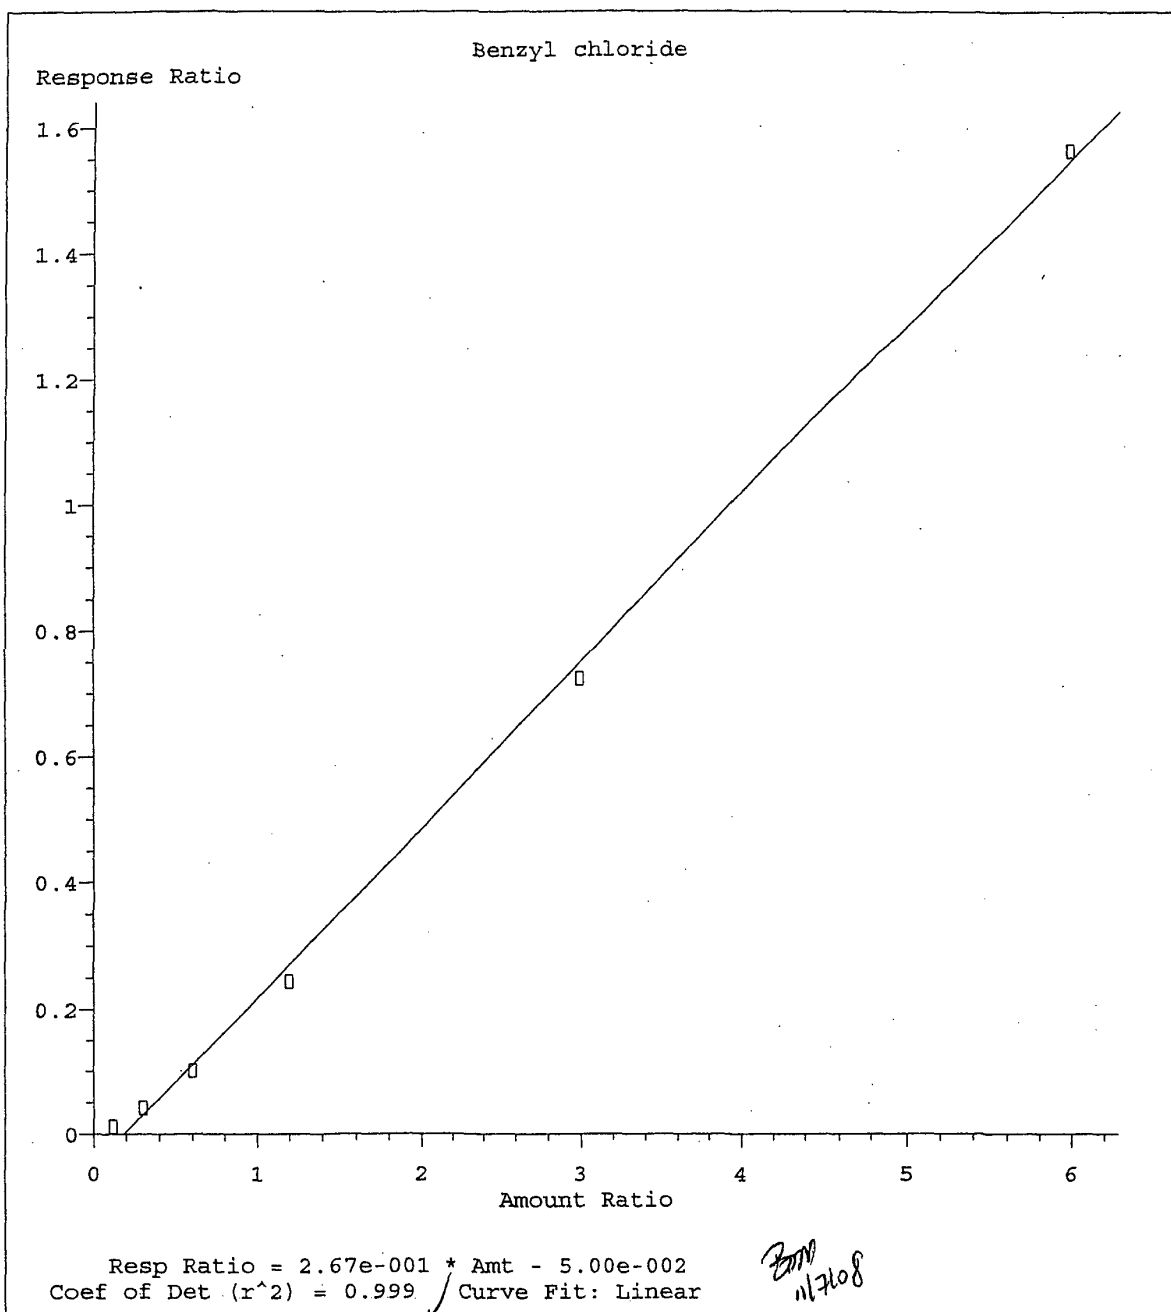

Method Name: H:\MSI.I\METHODS\I81104W.M
Calibration Table Last Updated: Fri Nov 07 14:59:59 2008

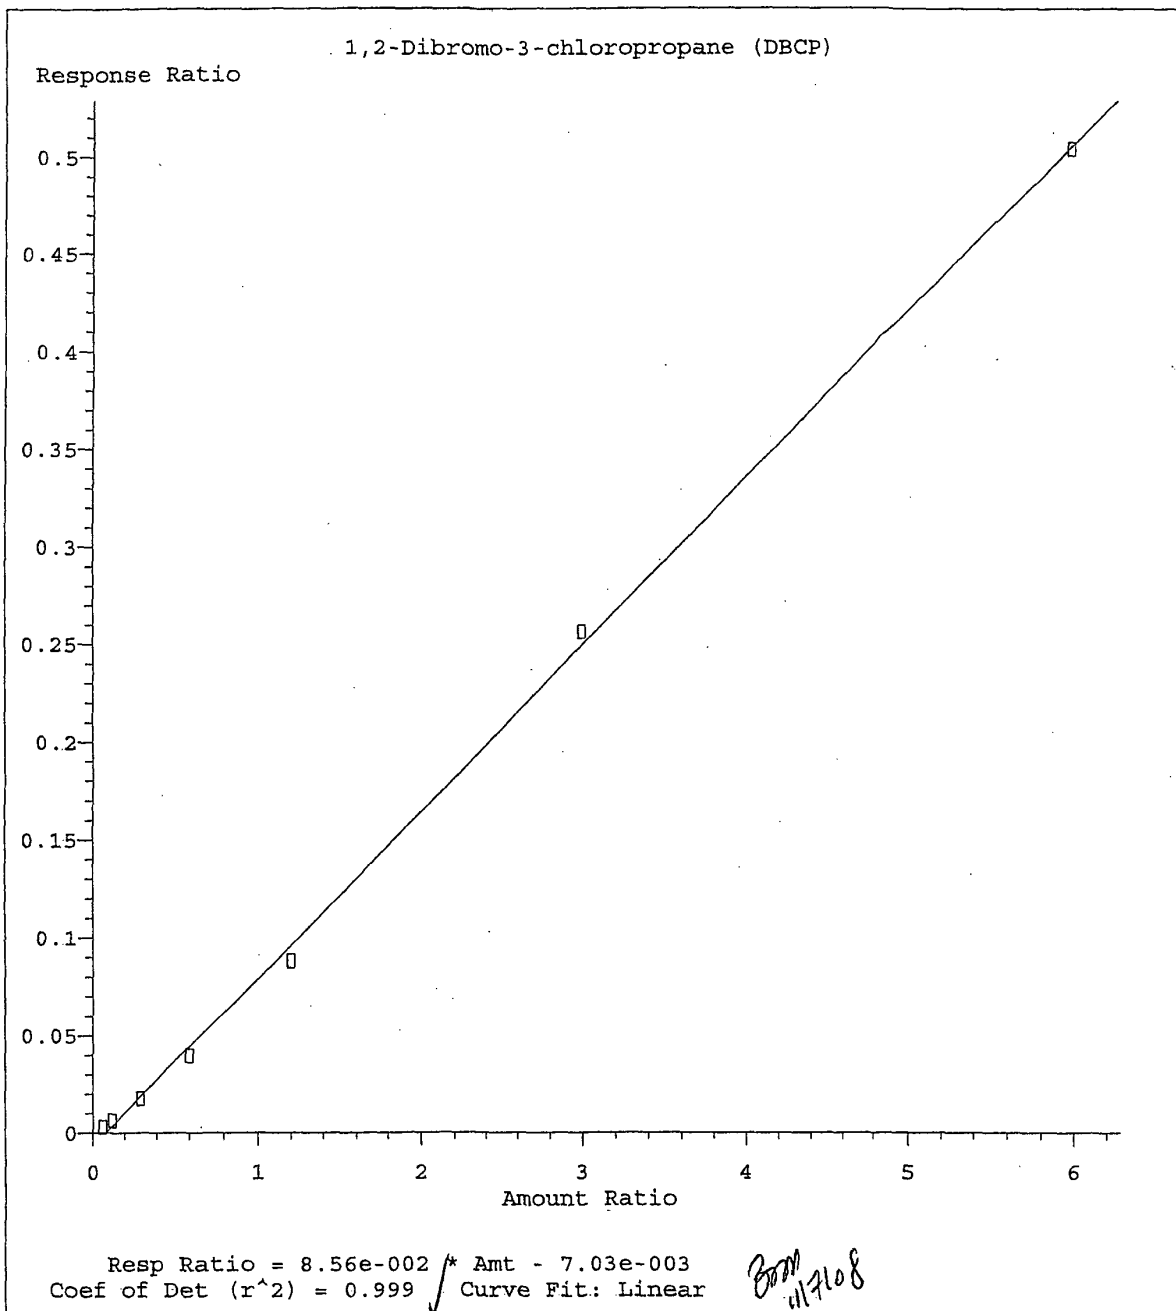

Method Name: H:\MSI.I\METHODS\I81104W.M
Calibration Table Last Updated: Fri Nov 07 15:01:14 2008

8260 ICV SUMMARY FORM (15 mL WATER)

Zam
11/10/08

IB04819.D								
	SPIKE	Result	ICV REC	ICV REC TOLERANCE				
COMPOUND	(ug/L)		%	LOW	HIGH	P/F	Analysis Date	File
Dichlorodifluoromethane	50	43.66	87.32	65	135		11/5/2008	IB04819.D
Chloromethane (SPCC)	50	36.90	73.80	65	135		11/5/2008	IB04819.D
Vinyl chloride (CCC)	50	44.62	89.24	65	135		11/5/2008	IB04819.D
Bromomethane	50	49.36	98.71	65	135		11/5/2008	IB04819.D
Ethylene oxide	625	497.71	79.63	65	135		11/6/2008	IB04826.D
Chloroethane	50	45.01	90.02	65	135		11/5/2008	IB04819.D
Trichlorofluoromethane	50	46.97	93.93	65	135		11/5/2008	IB04819.D
Ethyl ether	50	48.17	96.34	65	135		11/5/2008	IB04819.D
Ethanol	1250	1381.21	110.50	65	135		11/5/2008	IB04819.D
1,1-Dichloroethene (CCC)	50	48.28	96.55	65	135		11/5/2008	IB04819.D
Carbon disulfide	50	49.27	98.54	65	135		11/5/2008	IB04819.D
1,1,2-Trichlorotrifluoroethane	50	43.55	87.10	65	135		11/5/2008	IB04819.D
Propylene oxide	250	235.64	94.26	65	135		11/6/2008	IB04826.D
Iodomethane	50	50.66	101.31	65	135		11/5/2008	IB04819.D
Bromoethane	50	46.62	93.24	65	135		11/5/2008	IB04819.D
Acrolein	250	186.49	74.59	65	135		11/7/2008	IB04827.D
3-Chloropropene	50	45.58	91.15	65	135		11/5/2008	IB04819.D
Methylene chloride	50	48.44	96.87	65	135		11/5/2008	IB04819.D
Acetone	50	56.24	112.48	65	135		11/5/2008	IB04819.D
trans-1,2-Dichloroethene	50	50.15	100.30	65	135		11/5/2008	IB04819.D
Methyl acetate	125	119.88	95.90	65	135		11/6/2008	IB04826.D
Hexane	50	48.33	96.67	65	135		11/5/2008	IB04819.D
Methyl tert-butyl ether (MTBE)	50	50.71	101.41	65	135		11/5/2008	IB04819.D
tert-Butyl alcohol	1000	1155.75	115.58	65	135		11/5/2008	IB04819.D
Acetonitrile	250	251.62	100.65	65	135		11/5/2008	IB04819.D
Isopropyl ether	50	48.12	96.25	65	135		11/5/2008	IB04819.D
2-Chloro-1,3-butadiene	12.5	12.13	97.05	65	135		11/5/2008	IB04819.D
1,1-Dichloroethane (SPCC)	50	47.94	95.88	65	135		11/5/2008	IB04819.D
Acrylonitrile	250	263.36	105.35	65	135		11/5/2008	IB04819.D
Vinyl acetate	50	54.38	108.76	65	135		11/8/2008	IB08807.D
cis-1,2-Dichloroethene	50	51.22	102.44	65	135		11/5/2008	IB04819.D
2,2-Dichloropropane	50	49.53	99.05	65	135		11/5/2008	IB04819.D
Cyclohexane	50	48.15	96.31	65	135		11/5/2008	IB04819.D
Bromochloromethane	50	53.25	106.50	65	135		11/5/2008	IB04819.D
2-Methylhexane	50	NC	NC	65	135	NC	NC	NC
Chloroform (CCC)	50	50.24	100.48	65	135		11/5/2008	IB04819.D
Carbon tetrachloride	50	49.41	98.81	65	135		11/5/2008	IB04819.D
3-Methylhexane	50	NC	NC	65	135	NC	NC	NC
Ethyl acetate	250	270.18	108.07	65	135		11/5/2008	IB04819.D
Tetrahydrofuran	50	55.12	110.24	65	135		11/5/2008	IB04819.D
1,1,1-Trichloroethane	50	49.62	99.24	65	135		11/5/2008	IB04819.D
1,1-Dichloropropene	50	49.04	98.07	65	135		11/5/2008	IB04819.D
2-Butanone (MEK)	50	53.09	106.19	65	135		11/5/2008	IB04819.D
Benzene	50	49.41	98.82	65	135		11/5/2008	IB04819.D
Heptane	50	NC	NC	65	135	NC	NC	NC
Propionitrile	250	268.89	107.55	65	135		11/5/2008	IB04819.D
Methacrylonitrile	50	47.92	95.85	65	135		11/5/2008	IB04819.D
1,2-Dichloroethane	50	47.06	94.13	65	135		11/5/2008	IB04819.D
Isobutyl alcohol	1000	1031.46	103.15	65	135		11/5/2008	IB04819.D
Methylcyclohexane	125	115.56	92.45	65	135		11/6/2008	IB04826.D
Trichloroethene	50	48.83	97.67	65	135		11/5/2008	IB04819.D
Dibromomethane	50	52.82	105.64	65	135		11/5/2008	IB04819.D

8260 ICV SUMMARY FORM (15 mL WATER)

IB04819.D								
COMPOUND	SPIKE (ug/L)	Result	ICV REC %	ICV REC TOLERANCE		P/F	Analysis Date	File
				LOW	HIGH			
n-Butanol	2500	2582.29	103.29	65	135		11/5/2008	IB04819.D
1,2-Dichloropropane (CCC)	50	50.52	101.03	65	135		11/5/2008	IB04819.D
Bromodichloromethane	50	50.05	100.11	65	135		11/5/2008	IB04819.D
1,4-Dioxane	1000	1188.17	118.82	65	135		11/5/2008	IB04819.D
Methyl methacrylate	50	47.42	94.84	65	135		11/5/2008	IB04819.D
1-Bromo-2-chloroethane	50	50.04	100.08	65	135		11/5/2008	IB04819.D
cis-1,3-Dichloropropene	50	53.10	106.21	65	135		11/5/2008	IB04819.D
2-Chloroethyl vinyl ether	50	59.07	118.15	65	135		11/6/2008	IB04822.D
Toluene (CCC)	50	46.58	93.17	65	135		11/5/2008	IB04819.D
Epichlorohydrin	250	235.04	94.01	65	135		11/5/2008	IB04819.D
2-Nitropropane	100	109.39	109.39	65	135		11/6/2008	IB04825.D
Tetrachloroethane	50	49.07	98.14	65	135		11/5/2008	IB04819.D
4-Methyl-2-pentanone (MIBK)	50	54.94	109.88	65	135		11/5/2008	IB04819.D
trans-1,3-Dichloropropene	50	52.81	105.62	65	135		11/5/2008	IB04819.D
1,1,2-Trichloroethane	50	49.59	99.17	65	135		11/5/2008	IB04819.D
4-Methyl-2-pentanol (MIBC)	50	50.14	100.27	65	135		11/5/2008	IB04819.D
Ethyl methacrylate	50	47.54	95.08	65	135		11/5/2008	IB04819.D
Dibromochloromethane	50	54.81	109.61	65	135		11/5/2008	IB04819.D
1,3-Dichloropropane	50	49.46	98.91	65	135		11/5/2008	IB04819.D
1,2-Dibromoethane (EDB)	50	52.25	104.51	65	135		11/5/2008	IB04819.D
2-Hexanone	50	59.49	118.98	65	135		11/5/2008	IB04819.D
Chlorobenzene (SPCC)	50	48.66	97.32	65	135		11/5/2008	IB04819.D
1-Chlorohexane	50	48.19	96.38	65	135		11/5/2008	IB04819.D
Ethylbenzene (CCC)	50	48.01	96.01	65	135		11/5/2008	IB04819.D
1,1,1,2-Tetrachloroethane	50	51.39	102.77	65	135		11/5/2008	IB04819.D
m&p-Xylene	100	97.80	97.80	65	135		11/5/2008	IB04819.D
o-Xylene	50	49.68	99.37	65	135		11/5/2008	IB04819.D
Bromoform (SPCC)	50	60.58	121.15	65	135		11/5/2008	IB04819.D
Styrene	50	51.44	102.88	65	135		11/5/2008	IB04819.D
Isopropylbenzene	50	51.47	102.94	65	135		11/5/2008	IB04819.D
Bromobenzene	50	52.32	104.63	65	135		11/5/2008	IB04819.D
n-Propylbenzene	50	50.90	101.80	65	135		11/5/2008	IB04819.D
1,1,2,2-Tetrachloroethane (SPCC)	50	49.86	99.73	65	135		11/5/2008	IB04819.D
2-Chlorotoluene	50	49.15	98.31	65	135		11/5/2008	IB04819.D
Cyclohexanone	250	273.03	109.21	65	135		11/6/2008	IB04826.D
1,2,3-Trichloropropane	50	48.05	96.11	65	135		11/5/2008	IB04819.D
trans-1,4-Dichloro-2-butene	50	45.93	91.86	65	135		11/5/2008	IB04819.D
3-Ethyltoluene	50	47.96	95.92	65	135		11/5/2008	IB04819.D
4-Chlorotoluene	50	50.93	101.86	65	135		11/5/2008	IB04819.D
1,3,5-Trimethylbenzene	50	47.63	95.25	65	135		11/5/2008	IB04819.D
2-Ethyltoluene	50	47.69	95.37	65	135		11/5/2008	IB04819.D
tert-Butylbenzene	50	47.06	94.12	65	135		11/5/2008	IB04819.D
Pentachloroethane	50	54.02	108.03	65	135		11/5/2008	IB04819.D
1,2,4-Trimethylbenzene	50	47.68	95.36	65	135		11/5/2008	IB04819.D
sec-Butylbenzene	50	49.33	98.66	65	135		11/5/2008	IB04819.D
p-Isopropyltoluene	50	49.72	99.44	65	135		11/5/2008	IB04819.D
1,3-Dichlorobenzene	50	49.38	98.76	65	135		11/5/2008	IB04819.D

8260 ICV SUMMARY FORM (15 mL WATER)

IB04819.D								
	SPIKE	Result	ICV REC	ICV REC TOLERANCE				
COMPOUND	(ug/L)		%	LOW	HIGH	P/F	Analysis Date	File
1,4-Dichlorobenzene	50	46.88	93.76	65	135		11/5/2008	IB04819.D
Benzyl chloride	50	44.03	88.06	65	135		11/5/2008	IB04819.D
n-Butylbenzene	50	51.98	103.86	65	135		11/5/2008	IB04819.D
1,2-Dichlorobenzene	50	50.11	100.23	65	135		11/5/2008	IB04819.D
1,3,5-Trichlorobenzene	125	NC	NC	65	135	NC	NC	NC
1,2-Dibromo-3-chloropropane (DBCP)	50	54.24	108.48	65	135		11/5/2008	IB04819.D
Hexachlorobutadiene	50	45.09	90.18	65	135		11/5/2008	IB04819.D
1,2,4-Trichlorobenzene	50	53.58	107.16	65	135		11/5/2008	IB04819.D
Naphthalene	50	55.95	111.90	65	135		11/5/2008	IB04819.D
1,2,3-Trichlorobenzene	50	50.21	100.42	65	135		11/5/2008	IB04819.D
Dibromofluoromethane (Surr)	16.7	17.24	103.22	81	110		11/5/2008	IB04819.D
1,2-Dichloroethane-d4 (Surr)	16.7	15.19	90.94	75	115		11/5/2008	IB04819.D
Toluene-d8 (Surr)	16.7	17.28	103.49	90	114		11/5/2008	IB04819.D
1,4-Bromofluorobenzene (Surr)	16.7	15.66	93.79	86	117		11/5/2008	IB04819.D

Q = Failed criteria

NC = Not calibrated

Sequence Name: C:\HPCHEM\1\SEQUENCE\I110408.S
 Comment:
 Operator: dy
 Data Path: C:\HPCHEM\1\DATA\I110408.B\
 Pre-Seq Cmd:
 Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
 (X) Full Method (X) Inject Anyway
 () Reprocessing Only () Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Blank	1	IB04801	I81104W	BLANK, BLANK <i>BFB 11/106 11/1108</i>
2 Blank	2	IB04802	I81104W	BLANK, BLANK
3 Blank	3	IB04803	I81104W	BLANK, BLANK
4 Blank	4	IB04804	I81104W	BLANK, BLANK
5 Blank	5	IB04805	I81104W	STD 0.5ppb
6 Blank	6	IB04806	I81104W	STD 1ppb
7 Blank	7	IB04807	I81104W	STD 2ppb
8 Blank	8	IB04808	I81104W	STD 5ppb
9 Blank	9	IB04809	I81104W	STD 10ppb
10 Blank	10	IB04810	I81104W	STD 20ppb
11 Blank	11	IB04811	I81104W	STD 50ppb
12 Blank	12	IB04812	I81104W	STD 100ppb
13 Blank	13	IB04813	I81104W	BLANK, BLANK
14 Blank	14	IB04814	I81104W	BLANK, BLANK
15 Blank	15	IB04815	I81104W	BLANK, BLANK
16 Blank	16	IB04816	I81104W	BLANK, BLANK
17 Blank	17	IB04817	I81104W	NOT USED, special analyte mix - wrong <i>*recipe</i>
18 Blank	18	IB04818	I81104W	NOT USED, reactives mix
19 Blank	19	IB04819	I81104W	50ppb ICV; composite mix 17.26 <i>11/15/08</i>
20 Blank	20	IB04820	I81104W	BLANK, BLANK
21 Blank	21	IB04821	I81104W	BLANK, BLANK
22 Blank	22	IB04822	I81104W	50ppb ICV; reactives mix <i>Assemble out</i>
23 Blank	23	IB04823	I81104W	50ppb ICV; special analytes mi - <i>nocust</i>
24 Blank	24	IB04824	I81104W	BLANK, BLANK
25 Blank	25	IB04825	I81104W	50ppb ICV; MIX 5 10X ICV
26 Blank	26	IB04826	I81104W	50ppb ICV; special analytes mix
27 Blank	27	IB04827	I81104W	50ppb ICV; acrolein ICV 10x

Austin Laboratory

PAGE #: 21

INSTRUMENT GCMS-II

ANALYST / DATE: RA 11/4/08

SHIFT (Circle): 1 2 3

METHOD / TEST: 8260 - TICAL

COMPUTER CLOCK DATE / TIME: 14:06

SOP #: AU-MS-004, current revision

DAILY CHECK <u>✓</u>	COLUMN CHANGED <u>✓</u>	P&T MAINT. (Describe) <u>✓</u>	
M. PUMP OIL <u>✓</u>	TURBO OIL <u>✓</u>	FILAMENT CHANGE <u>✓</u>	OTHER <u>NA</u>

DAILY CHECK includes sufficient carrier and detector gases, correct column flow/pressure, etc. Column and gases changed as needed. Source cleaned as needed. Mechanical pump oil and turbomolecular pump oil changed semiannually (usually on service contract). OTHER is for minor maintenance performed or for reference to Repair Log for major repairs.

MASS SPECTROMETER CONDITIONS:

Tune File: Atune.u Sampling Rate 2^{m} 4
 Elect Mult. 1224 volts Scan Range 35-300 amu
 Tuning Performance: BFB Interface: Open-Split

GC PROGRAM:

GC Meth. 81104.u Init. Hold 2 min 2nd Temp 210 C
 Inj. Temp 150 C Ramp 9 C/min 2nd Hold 4 min
 Carrier Gas: Helium Final Temp. 85 C 3rd Ramp C/min
 Flow/Pressure 1.3 Final Hold 0 min 3rd Temp C
 Initial Temp. 35 C 2nd Ramp 30 C/min 3rd Hold min

GC COLUMN:


Column ID#: MSVOAID 010 Capillary
 Phases/Loadings: RTXVMS i.d. 0.25 mm Length 30 m
 Injection Type (Circle & Describe): Purge & Trap Tekmar Velocity/Solatek
 Split 120:1 Splitless

INSTRUMENT SEQUENCE:

1 Blank	1 IB04801	I81104W	BLANK, BLANK	BFB 14:06 11/4/08	
2 Blank	2 IB04802	I81104W	BLANK, BLANK		
3 Blank	3 IB04803	I81104W	BLANK, BLANK	} not used - stabilizing blanks	
4 Blank	4 IB04804	I81104W	BLANK, BLANK		
5 Blank	5 IB04805	I81104W	STD 0.5ppb		
6 Blank	6 IB04806	I81104W	STD 1ppb		
7 Blank	7 IB04807	I81104W	STD 2ppb		
8 Blank	8 IB04808	I81104W	STD 5ppb		
9 Blank	9 IB04809	I81104W	STD 10ppb		
10 Blank	10 IB04810	I81104W	STD 20ppb		
11 Blank	11 IB04811	I81104W	STD 50ppb		
12 Blank	12 IB04812	I81104W	STD 100ppb		
13 Blank	13 IB04813	I81104W	BLANK, BLANK	} not used - cleanup / system blanks	
14 Blank	14 IB04814	I81104W	BLANK, BLANK		
15 Blank	15 IB04815	I81104W	BLANK, BLANK		
16 Blank	16 IB04816	I81104W	BLANK, BLANK		
17 Blank	17 IB04817	I81104W	NOT USED, special analyte mix - wrong recipe		
18 Blank	18 IB04818	I81104W	NOT USED, reactives mix		
19 Blank	19 IB04819	I81104W	50ppb ICV; composite mix	17.26 11/5/08	
20 Blank	20 IB04820	I81104W	BLANK, BLANK	} not used - system blanks	
21 Blank	21 IB04821	I81104W	BLANK, BLANK		
22 Blank	22 IB04822	I81104W	50ppb ICV; reactives mix	Analyte out	
23 Blank	23 IB04823	I81104W	50ppb ICV; special analytes mix	11/11/08	
24 Blank	24 IB04824	I81104W	BLANK, BLANK	not used - system blanks	
25 Blank	25 IB04825	I81104W	50ppb ICV; MIX 5 10X ICV		
26 Blank	26 IB04826	I81104W	50ppb ICV; special analytes mix		
27 Blank	27 IB04827	I81104W	50ppb ICV; acrolein ICV 10x		

BFB

Data File : C:\HPCHEM\1\DATA\I110408.B\IB04801.D Vial: 1
 Acq On : 4 Nov 2008 2:06 pm Operator: kma
 Sample : BLANK;BLANK Inst : MSI
 Misc : 1,1, 08MSV0798 IS 08MSV0682 SUR Multiplr: 1.00
 MS Integration Params: VOA.P
 Method : C:\HPCHEM\1\METHODS\I80916W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water

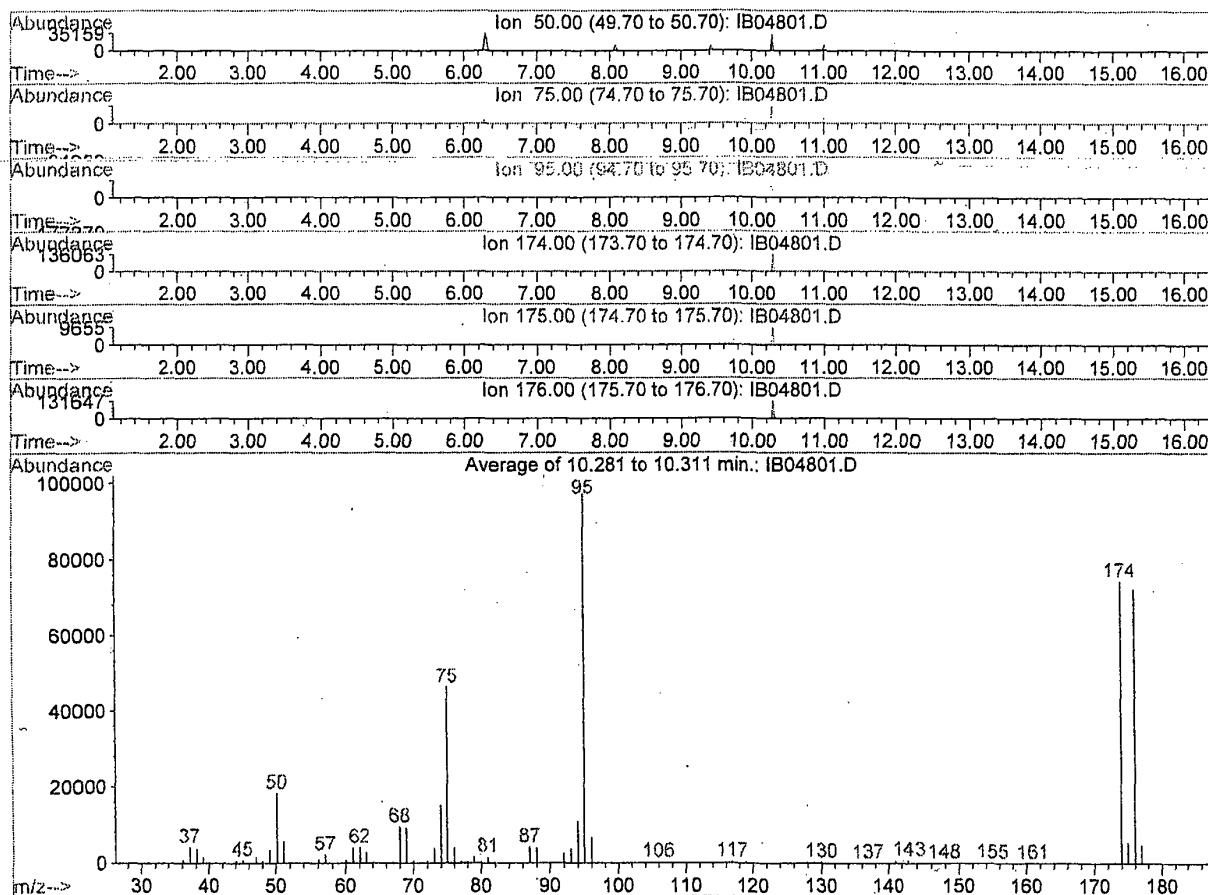

Spectrum Information: Average of 10.281 to 10.311 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	18377	PASS
75	95	30	60	47.8	46417	PASS
95	95	100	100	100.0	97040	PASS
96	95	5	9	6.9	6674	PASS
173	174	0.00	2	0.5	378	PASS
174	95	50	100	76.8	74575	PASS
175	174	5	9	7.2	5394	PASS
176	174	95	101	97.0	72327	PASS
177	176	5	9	6.5	4686	PASS

Injection Log

Directory: h:\msi\i110408.b

K-A 11/12/08

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	1	ib04801.d	1.	BLANK;BLANK	1,1, 08MSV0798 IS 08MSV0682 SUR	4 Nov 08 14:06
2	2	ib04802.d	1.	BLANK;BLANK	1,1, 08MSV0798 IS	4 Nov 08 14:33
3	3	ib04803.d	1.	BLANK;BLANK	1,1, 08MSV0798 IS	4 Nov 08 14:57
4	4	ib04804.d	1.	BLANK;BLANK	1,1, 08MSV0798 IS	4 Nov 08 15:24
5	5	ib04805.d	1.	STD 0.5ppb	1,1, 0.5uL/50mL 08MSV0802	4 Nov 08 15:51
6	6	ib04806.d	1.	STD 1ppb	1,1, 1uL/50mL 08MSV0802	4 Nov 08 16:20
7	7	ib04807.d	1.	STD 2ppb	1,1, 2uL/50mL 08MSV0802	4 Nov 08 16:47
8	8	ib04808.d	1.	STD 5ppb	1,1, 5uL/50mL 08MSV0802	4 Nov 08 17:14
9	9	ib04809.d	1.	STD 10ppb	1,1, 10uL/50mL 08MSV0802	4 Nov 08 17:41
10	10	ib04810.d	1.	STD 20ppb	1,1, 20uL/50mL 08MSV0802	4 Nov 08 18:08
11	11	ib04811.d	1.	STD 50ppb	1,1, 50uL/50mL 08MSV0802	4 Nov 08 18:35
12	12	ib04812.d	1.	STD 100ppb	1,1, 100uL/50mL 08MSV0802	4 Nov 08 19:02
13	13	ib04813.d	1.	BLANK;BLANK	1,1, 08MSV0798 IS	4 Nov 08 19:28
14	14	ib04814.d	1.	BLANK;BLANK	1,1, 08MSV0798 IS	4 Nov 08 19:56
15	15	ib04815.d	1.	BLANK;BLANK	1,1, 08MSV0798 IS 08MSV0682 SUR	5 Nov 08 14:16
16	16	ib04816.d	1.	BLANK;BLANK	1,1, 08MSV0798 IS 08MSV0682 SUR	5 Nov 08 14:43
17	17	ib04817.d	1.	NOT USED;special analyte mix	1,1, 12.5uL/50mL 08MSV0818	5 Nov 08 16:31
18	18	ib04818.d	1.	50 PPB ICV;reactives mix,RC	1,1, 12.5uL/50mL 08MSV0817	5 Nov 08 16:58
19	19	ib04819.d	1.	50ppb ICV;composite mix,COMP	1,1, 12.5uL/50mL 08MSV0816	5 Nov 08 17:26
20	20	ib04820.d	1.	BLANK;BLANK	1,1, 08MSV0798 IS 08MSV0682 SUR	6 Nov 08 10:49
21	21	ib04821.d	1.	BLANK;BLANK	1,1, 08MSV0798 IS 08MSV0682 SUR	6 Nov 08 11:16
22	22	ib04822.d	1.	50ppb ICV;reactives mix,RC	1,1, 12.5/50 08MSV0819/810 25/50 08MSV0	6 Nov 08 11:43
23	23	ib04823.d	1.	50ppb ICV;special analytes mix,SPECIAL	1,1, 12.5/50 08MSV0820	6 Nov 08 12:10
24	24	ib04824.d	1.	BLANK;BLANK	1,1, 08MSV0798 IS 08MSV0682 SUR	6 Nov 08 15:12
25	25	ib04825.d	1.	50ppb ICV;MIX 5 10X ICV,MIX5	1,1, 12.5uL/50mL 08MSV0822	6 Nov 08 15:39
26	26	ib04826.d	1.	50ppb ICV;special analytes mix,SPECIAL	1,1, 12.5uL/50mL 08MSV0821	6 Nov 08 16:07
27	27	ib04827.d	1.	50ppb ICV;acrolein ICV 10x,RC	1,1, 12.5uL/50mL 08MSV0824	7 Nov 08 07:54

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04805.D
 Acq On : 4 Nov 2008 3:51 pm
 Sample : STD 0.5ppb
 Misc : 1,1, 0.5uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 7 13:59 19108

Vial: 5
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	712521	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.43	119	142601	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.01	152	186238	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	5406	0.5759	PPB	0.00
Spiked Amount	16.700		Recovery	=	3.47%	
50) 1,2-Dichloroethane-d4 (Sur)	6.00	67	3561	0.7360	PPB	0.00
Spiked Amount	16.700		Recovery	=	4.43%	
64) Toluene-d8 (Surr)	8.09	98	21017	0.5178	PPB	0.00
Spiked Amount	16.700		Recovery	=	3.11%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	7266	0.5714	PPB	0.00
Spiked Amount	16.700		Recovery	=	3.41%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.59	85	9406	0.6403	PPB	100
3) Chloromethane (SPCC)	1.78	50	8355	0.4340	PPB	97
4) Vinyl chloride (CCC)	1.87	62	9505	0.5487	PPB	98
5) Bromomethane	2.19	94	6207	0.7316	PPB	98
6) Ethylene oxide	2.29	44	11755	10.2730	PPB	96
7) Chloroethane	2.32	64	6593	0.5852	PPB	97
8) Trichlorofluoromethane	2.48	101	10532	0.6550	PPB	98
9) Ethyl ether	2.80	59	4845	0.6754	PPB	95
11) 1,1-Dichloroethene (CCC)	2.99	96	6111	0.6010	PPB	97
12) Carbon disulfide	3.01	76	20562	0.5532	PPB	94
13) 1,1,2-Trichlorotrifluoroet	3.05	101	6170	0.6169	PPB	98
14) Propylene oxide	3.13	58	3146	3.1194	PPB	98
16) Bromoethane	3.25	108	4730	0.5562	PPB	95
17) Acrolein	3.35	56	1371	2.1608	PPB	95
18) 3-Chloropropene	3.48	41	11404	0.5433	PPB	96
19) Methylene chloride	3.59	84	7026	0.6543	PPB	94
20) Acetone	3.67	58	204	0.5384	PPB	# 1
21) trans-1,2-Dichloroethene	3.75	96	6816	0.6007	PPB	98
22) Methyl acetate	3.79	74	1100	1.3582	PPB	# 59
23) Hexane	3.84	86	2287	0.5491	PPB	# 82
24) Methyl tert-butyl ether (M)	3.87	73	12936	0.6419	PPB	94
25) tert-Butyl alcohol	3.99	59	5558	30.1905	PPB	75
26) Acetonitrile	4.12	40	1228	5.3091	PPB	84
27) Isopropyl ether	4.27	45	23137	0.6098	PPB	95
28) 2-Chloro-1,3-butadiene	4.36	88	4564	0.4740	PPB	91
29) 1,1-Dichloroethane (SPCC)	4.39	63	13135	0.6020	PPB	100
30) Acrylonitrile	4.45	53	5767	3.6554	PPB	97
31) Vinyl acetate	4.67	43	6443	0.5394	PPB	94
32) cis-1,2-Dichloroethene	4.95	96	6881	0.5800	PPB	94
33) 2,2-Dichloropropane	5.05	77	9456	0.5533	PPB	90
34) Cyclohexane	5.15	56	12678	0.5898	PPB	94
35) Bromochloromethane	5.16	130	3145	0.6000	PPB	87
37) Chloroform (CCC)	5.25	83	11181	0.6228	PPB	96
38) Carbon tetrachloride	5.38	117	7525	0.5834	PPB	99

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 TR04805.D I81104W.M Fri Nov 07 14:20:57 2008 RPT1

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04805.D
 Acq On : 4 Nov 2008 3:51 pm
 Sample : STD 0.5ppb
 Misc : 1,1, 0.5uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 7 13:59 19108

Vial: 5
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
40) Ethyl acetate	5.38	43	14307	3.4076	PPB	96
43) 1,1,1-Trichloroethane	5.44	97	9337	0.6015	PPB	96
44) 1,1-Dichloropropene	5.58	75	8819	0.5638	PPB	97
45) 2-Butanone (MEK)	5.58	43	1508	0.9319	PPB	67
46) Benzene	5.85	78	28224	0.5734	PPB	98
48) Propanenitrile	5.89	54	1950	3.6107	PPB	83
49) Methacrylonitrile	5.90	67	6455	3.0002	PPB	92
51) 1,2-Dichloroethane	6.06	62	7122	0.7129	PPB	98
52) Isobutyl alcohol	6.14	43	2285	25.9375	PPB	87
53) Methylcyclohexane	6.47	83	21967	1.0772	PPB	96
54) Trichloroethene	6.50	130	6759	0.5805	PPB	97
55) Dibromomethane	6.97	93	2392	0.6472	PPB	94
56) n-Butanol	6.94	56	2151	88.1889	PPB	87
57) 1,2-Dichloropropane (CCC)	7.09	63	6633	0.6088	PPB	84
58) Bromodichloromethane	7.17	83	7128	0.5970	PPB	90
59) 1,4-Dioxane	7.43	88	557	34.2332	PPB #	52
60) Methyl methacrylate	7.37	69	1689	0.4704	PPB	97
61) 1-Bromo-2-chloroethane	7.73	63	6820	0.6473	PPB #	96
62) cis-1,3-Dichloropropene	7.90	75	7953	0.5070	PPB	99
63) 2-Chloroethyl vinyl ether	7.85	63	1150	0.3610	PPB	80
66) Toluene (CCC)	8.14	91	26162	0.5711	PPB	98
67) Epichlorohydrin	8.17	57	1204	3.7268	PPB	72
68) 2-Nitropropane	8.36	43	453	0.3936	PPB #	86
69) Tetrachloroethene	8.50	164	4725	0.5897	PPB	99
70) 4-Methyl-2-pentanone (MIBK)	8.52	43	2118	0.5849	PPB	89
71) trans-1,3-Dichloropropene	8.55	75	5700	0.5365	PPB	92
72) 1,1,2-Trichloroethane	8.69	97	3368	0.6394	PPB	86
73) 4-Methyl-2-pentanol (MIBC)	8.63	45	1353	3.3218	PPB	82
74) Ethyl methacrylate	8.70	69	2914	0.4240	PPB	91
75) Dibromochloromethane	8.84	129	3373	0.5882	PPB	98
76) 1,3-Dichloropropane	8.92	76	7653	0.7259	PPB	95
77) 1,2-Dibromoethane (EDB)	9.02	107	3062	0.6650	PPB	96
79) Chlorobenzene (SPCC)	9.44	112	17347	0.6260	PPB	81
80) 1-Chlorohexane	9.43	55	10857	1.0041	PPB	71
81) Ethylbenzene (CCC)	9.46	106	9562	0.5817	PPB #	84
82) 1,1,1,2-Tetrachloroethane	9.49	131	4650	0.5655	PPB	92
83) m&p-Xylene	9.57	106	22350	1.0903	PPB	95
84) o-Xylene	9.88	106	9898	0.5153	PPB	95
85) Bromoform (SPCC)	9.94	173	1400	0.5016	PPB	88
86) Styrene	9.92	104	12255	0.4298	PPB	99
87) Isopropylbenzene	10.10	105	23665	0.5238	PPB	99
88) Bromobenzene	10.36	156	5028	0.5444	PPB #	86
89) n-Propylbenzene	10.38	120	6305	0.4709	PPB #	81
90) 1,1,2,2-Tetrachloroethane	10.43	83	3566	0.6938	PPB	97
93) 2-Chlorotoluene	10.48	126	5818	0.5376	PPB	90
95) 1,2,3-Trichloropropane	10.52	110	1237	0.7789	PPB	91
96) trans-1,4-Dichloro-2-buten	10.54	53	640	0.4544	PPB #	52
97) 3-Ethyltoluene	10.43	105	23399	0.5107	PPB	97
98) 4-Chlorotoluene	10.59	126	5725	0.5321	PPB	86

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04805.D I81104W.M Fri Nov 07 14:20:58 2008 RPT1

Quantitation Report (QT Reviewed)

90/132

Data File : H:\MSI.I\I110408.B\IB04805.D Vial: 5
 Acq On : 4 Nov 2008 3:51 pm Operator: kma
 Sample : STD 0.5ppb Inst : MSI
 Misc : 1,1, 0.5uL/50mL 08MSV0802 Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Nov 7 13:59 19108 Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
99) 1,3,5-Trimethylbenzene	10.50	105	20071	0.5202	PPB	68
100) 2-Ethyltoluene	10.64	105	24341	0.5319	PPB	75
101) tert-Butylbenzene	10.71	91	11750	0.5589	PPB	81
102) Pentachloroethane	10.73	167	2385	0.4629	PPB	86
103) 1,2,4-Trimethylbenzene	10.75	105	19437	0.5049	PPB	98
104) sec-Butylbenzene	10.82	105	26193	0.5479	PPB	97
105) p-Isopropyltoluene	10.90	119	20566	0.4934	PPB	98
106) 1,3-Dichlorobenzene	10.96	146	10809	0.5846	PPB	99
107) 1,4-Dichlorobenzene	11.02	146	11850	0.6157	PPB	82
109) n-Butylbenzene	11.16	134	4807	0.4552	PPB	96
110) 1,2-Dichlorobenzene	11.28	146	8742	0.5943	PPB	98
112) 1,2-Dibromo-3-chloropropan	11.75	157	278	2.5565	PPB #	76
113) Hexachlorobutadiene	12.11	225	2708	0.4792	PPB	98
114) 1,2,4-Trichlorobenzene	12.14	180	4257	0.4836	PPB	98
115) Naphthalene	12.32	128	5006	0.4189	PPB	99
116) 1,2,3-Trichlorobenzene	12.43	180	3077	0.5169	PPB	97

 (#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 TR04805.D I81104W.M Fri Nov 07 14:20:58 2008 RPT1


Quantitation Report

Data File : C:\HPCHEM\1\DATA\I110408.B\IB04805.D
 Acq On : 4 Nov 2008 3:51 pm
 Sample : STD 0.5ppb
 Misc : 1,1, 0.5uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 16:07 19108

Vial: 5
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration

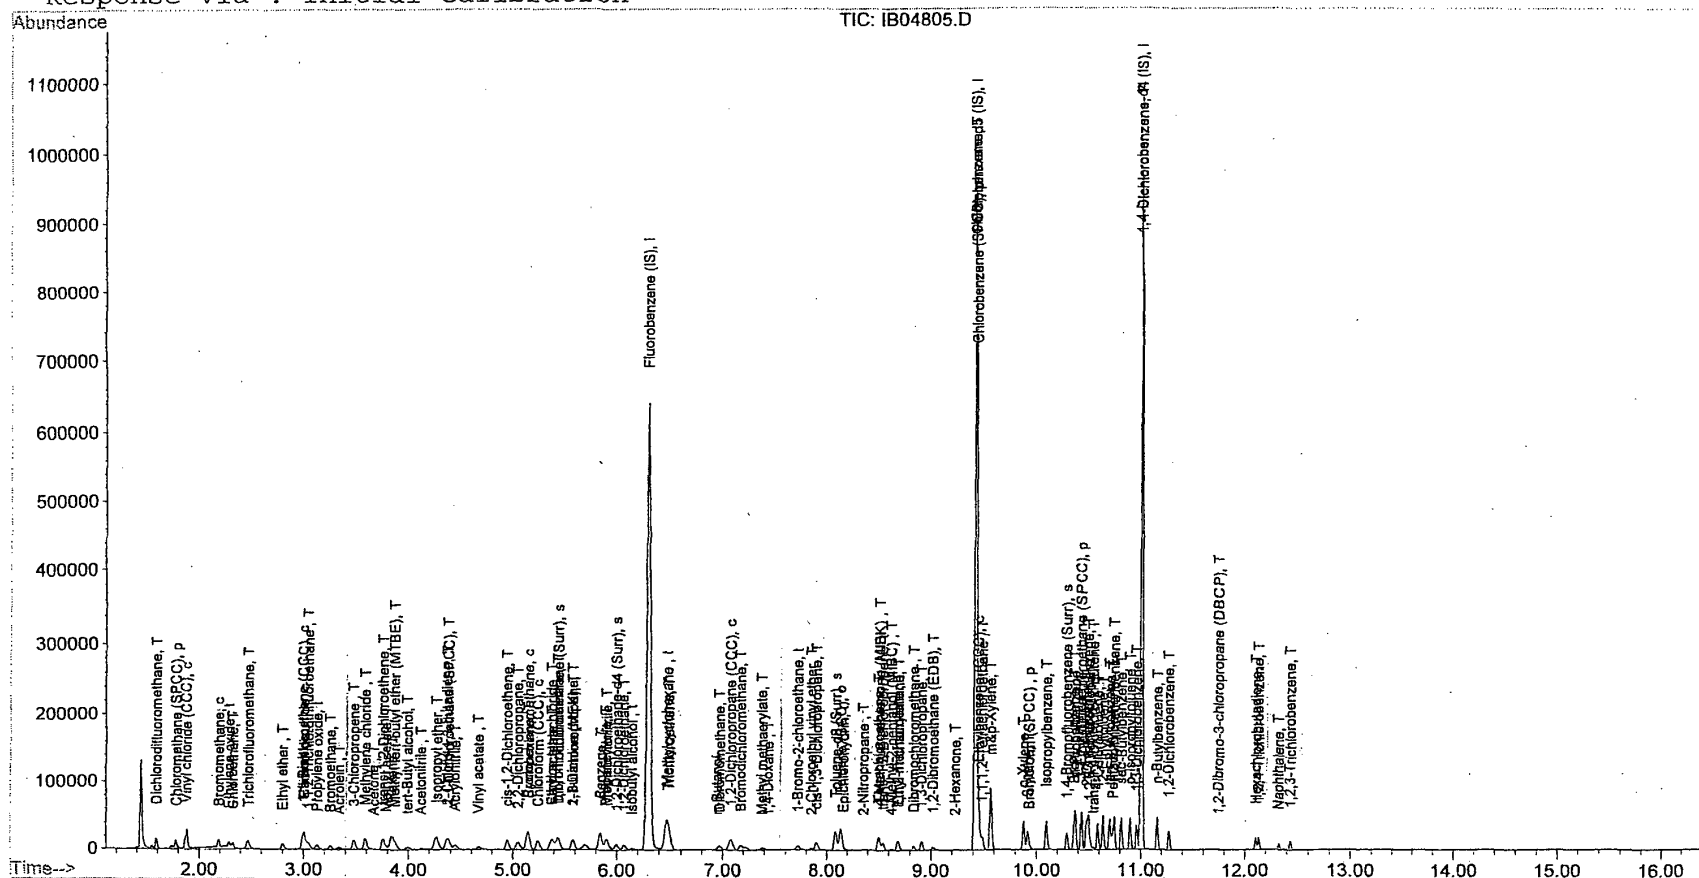

Quantitation Report (QT Reviewed) *KA*

Data File : H:\MSI.I\I110408.B\IB04806.D
 Acq On : 4 Nov 2008 4:20 pm
 Sample : STD 1ppb
 Misc : 1,1, 1uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 5 11:34 19108

Vial: 6 *NOV 06 2008*
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	712992	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.43	119	142545	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.01	152	187862	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	10353	1.1022	PPB	0.00
Spiked Amount	16.700		Recovery	=	6.59%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	6645	1.3725	PPB	0.00
Spiked Amount	16.700		Recovery	=	8.20%	
64) Toluene-d8 (Surr)	8.09	98	39966	0.9840	PPB	0.00
Spiked Amount	16.700		Recovery	=	5.87%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	13665	1.0750	PPB	0.00
Spiked Amount	16.700		Recovery	=	6.41%	
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	1.59	85	16545	1.1255	PPB	98
3) Chloromethane (SPCC)	1.77	50	15488	0.8040	PPB	96
4) Vinyl chloride (CCC)	1.86	62	17403	1.0039	PPB	93
5) Bromomethane	2.19	94	10758	1.2671	PPB	99
6) Ethylene oxide	2.29	44	18165	15.8643	PPB	92
7) Chloroethane	2.32	64	12462	1.1054	PPB	98
8) Trichlorofluoromethane	2.47	101	18339	1.1398	PPB	99
9) Ethyl ether	2.80	59	9006	1.2546	PPB	95
10) Ethanol	2.98	45	1401	63.2878	PPB	# 70
11) 1,1-Dichloroethene (CCC)	2.99	96	10947	1.0759	PPB	96
12) Carbon disulfide	3.01	76	36120	0.9712	PPB	96
13) 1,1,2-Trichlorotrifluoroet	3.04	101	11138	1.1129	PPB	98
14) Propylene oxide	3.12	58	6185	6.1286	PPB	98
15) Iodomethane	3.12	142	5937	0.3661	PPB	97
16) Bromoethane	3.25	108	8771	1.0307	PPB	100
17) Acrolein	3.35	56	2819	4.4401	PPB	97
18) 3-Chloropropene	3.48	41	20897	0.9949	PPB	97
19) Methylene chloride	3.59	84	12853	1.1962	PPB	98
20) Acetone	3.65	58	484	1.2766	PPB	# 1
21) trans-1,2-Dichloroethene	3.76	96	11841	1.0429	PPB	94
22) Methyl acetate	3.79	74	2226	2.7466	PPB	# 79
23) Hexane	3.83	86	4034	0.9680	PPB	# 80
24) Methyl tert-butyl ether (M)	3.87	73	25459	1.2624	PPB	88
25) tert-Butyl alcohol	3.99	59	11659	63.2886	PPB	80
26) Acetonitrile	4.12	40	2164	9.3496	PPB	# 79
27) Isopropyl ether	4.27	45	44164	1.1632	PPB	98

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04806.D I81104W.M Thu Nov 06 11:53:24 2008 KMA Page 1

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04806.D
 Acq On : 4 Nov 2008 4:20 pm
 Sample : STD lppb
 Misc : 1,1, 1uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 5 11:34 19108

Vial: 6
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
28) 2-Chloro-1,3-butadiene	4.36	88	8278	0.8592	PPB	87
29) 1,1-Dichloroethane (SPCC)	4.38	63	24221	1.1094	PPB	99
30) Acrylonitrile	4.44	53	11261	7.1330	PPB	100
31) Vinyl acetate	4.66	43	12414	1.0385	PPB	95
32) cis-1,2-Dichloroethene	4.95	96	12431	1.0471	PPB	97
33) 2,2-Dichloropropane	5.05	77	18049	1.0554	PPB	94
34) Cyclohexane	5.15	56	22230	1.0335	PPB	94
35) Bromochloromethane	5.15	130	5981	1.1404	PPB	90
37) Chloroform (CCC)	5.25	83	20820	1.1589	PPB	98
38) Carbon tetrachloride	5.37	117	13751	1.0655	PPB	99
40) Ethyl acetate	5.39	43	27807	6.6186	PPB	97
41) Tetrahydrofuran	5.42	72	559	0.8866	PPB	# 29
43) 1,1,1-Trichloroethane	5.44	97	17099	1.1009	PPB	98
44) 1,1-Dichloropropene	5.57	75	16057	1.0259	PPB	96
45) 2-Butanone (MEK)	5.58	43	2984	1.8428	PPB	63
46) Benzene	5.84	78	51710	1.0498	PPB	99
48) Propanenitrile	5.88	54	4045	7.4850	PPB	96
49) Methacrylonitrile	5.90	67	12310	5.7177	PPB	88
51) 1,2-Dichloroethane	6.07	62	13056	1.3059	PPB	100
52) Isobutyl alcohol	6.14	43	4547	51.5799	PPB	87
53) Methylcyclohexane	6.47	83	39700	1.9456	PPB	96
54) Trichloroethene	6.50	130	11803	1.0130	PPB	93
55) Dibromomethane	6.97	93	4339	1.1731	PPB	95
56) n-Butanol	6.94	56	4679	134.4027	PPB	88
57) 1,2-Dichloropropane (CCC)	7.08	63	11945	1.0956	PPB	89
58) Bromodichloromethane	7.17	83	13050	1.0924	PPB	95
59) 1,4-Dioxane	7.42	88	1151	70.6936	PPB	93
60) Methyl methacrylate	7.38	69	3070	0.8544	PPB	80
61) 1-Bromo-2-chloroethane	7.72	63	12999	1.2329	PPB	97
62) cis-1,3-Dichloropropene	7.90	75	15318	0.9759	PPB	96
63) 2-Chloroethyl vinyl ether	7.86	63	2535	0.7952	PPB	90
66) Toluene (CCC)	8.14	91	49824	1.0880	PPB	98
67) Epichlorohydrin	8.16	57	2187	6.7722	PPB	# 18
68) 2-Nitropropane	8.37	43	949	0.8248	PPB	88
69) Tetrachloroethene	8.51	164	8229	1.0275	PPB	95
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	4276	1.1812	PPB	93
71) trans-1,3-Dichloropropene	8.54	75	11148	1.0497	PPB	98
72) 1,1,2-Trichloroethane	8.69	97	6715	1.2753	PPB	93
73) 4-Methyl-2-pentanol (MIBC)	8.62	45	2814	6.9114	PPB	73
74) Ethyl methacrylate	8.70	69	5826	0.8480	PPB	92
75) Dibromochloromethane	8.84	129	6510	1.1356	PPB	95

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04806.D I81104W.M Thu Nov 06 11:53:25 2008 KMA Page 2

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04806.D
 Acq On : 4 Nov 2008 4:20 pm
 Sample : STD 1ppb
 Misc : 1,1, 1uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 5 11:34 19108

Vial: 6
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
76) 1,3-Dichloropropane	8.91	76	13900	1.3189	PPB	94
77) 1,2-Dibromoethane (EDB)	9.02	107	5764	1.2523	PPB	97
78) 2-Hexanone	9.22	43	2376	1.1299	PPB	89
79) Chlorobenzene (SPCC)	9.44	112	31018	1.1199	PPB	88
80) 1-Chlorohexane	9.43	55	15982	1.4322	PPB	82
81) Ethylbenzene (CCC)	9.46	106	16903	1.0286	PPB	# 83
82) 1,1,1,2-Tetrachloroethane	9.49	131	9127	1.1104	PPB	94
83) m&p-Xylene	9.57	106	41504	2.0254	PPB	94
84) o-Xylene	9.88	106	18837	0.9810	PPB	94
85) Bromoform (SPCC)	9.94	173	2730	0.9784	PPB	94
86) Styrene	9.92	104	23747	0.8331	PPB	96
87) Isopropylbenzene	10.09	105	45015	0.9968	PPB	98
88) Bromobenzene	10.36	156	9320	1.0095	PPB	# 87
89) n-Propylbenzene	10.37	120	12129	0.9061	PPB	# 82
90) 1,1,2,2-Tetrachloroethane	10.43	83	7023	1.3669	PPB	97
93) 2-Chlorotoluene	10.48	126	11002	1.0078	PPB	88
94) Cyclohexanone	10.54	42	341	8.5726	PPB	# 65
95) 1,2,3-Trichloropropane	10.52	110	2376	1.4832	PPB	99
96) trans-1,4-Dichloro-2-buten	10.54	53	1305	0.9186	PPB	72
97) 3-Ethyltoluene	10.43	105	45075	0.9754	PPB	98
98) 4-Chlorotoluene	10.59	126	10636	0.9801	PPB	88
99) 1,3,5-Trimethylbenzene	10.50	105	38749	0.9956	PPB	69
100) 2-Ethyltoluene	10.64	105	47269	1.0241	PPB	75
101) tert-Butylbenzene	10.70	91	22202	1.0469	PPB	82
102) Pentachloroethane	10.73	167	4644	0.8936	PPB	85
103) 1,2,4-Trimethylbenzene	10.75	105	39102	1.0070	PPB	97
104) sec-Butylbenzene	10.82	105	48605	1.0079	PPB	97
105) p-Isopropyltoluene	10.90	119	39995	0.9512	PPB	98
106) 1,3-Dichlorobenzene	10.96	146	19770	1.0600	PPB	98
107) 1,4-Dichlorobenzene	11.01	146	21459	1.1054	PPB	88
108) Benzyl chloride	11.16	126	1023	0.4190	PPB	# 1
109) n-Butylbenzene	11.16	134	8825	0.8285	PPB	91
110) 1,2-Dichlorobenzene	11.27	146	16413	1.1062	PPB	98
112) 1,2-Dibromo-3-chloropropan	11.76	157	551	2.8898	PPB	# 68
113) Hexachlorobutadiene	12.11	225	5254	0.9218	PPB	97
114) 1,2,4-Trichlorobenzene	12.14	180	8525	0.9602	PPB	95
115) Naphthalene	12.33	128	10727	0.8898	PPB	99
116) 1,2,3-Trichlorobenzene	12.44	180	6195	1.0316	PPB	99

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04806.D I81104W.M Thu Nov 06 11:53:25 2008 KMA Page 3


Quantitation report

Data File : C:\HPCHEM\1\DATA\I110408.B\IB04806.D
Acq On : 4 Nov 2008 4:20 pm
Sample : STD lppb
Misc : 1,1, 1uL/50mL 08MSV0802
MS Integration Params: VOA.P
Quant Time: Nov 4 16:36 19108

Vial: 6
Operator: kma
Inst : MSI
Multiplr: 1.00

Quant Results File: I81104W.RES

Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Wed Sep 24 14:27:06 2008
Response via : Initial Calibration

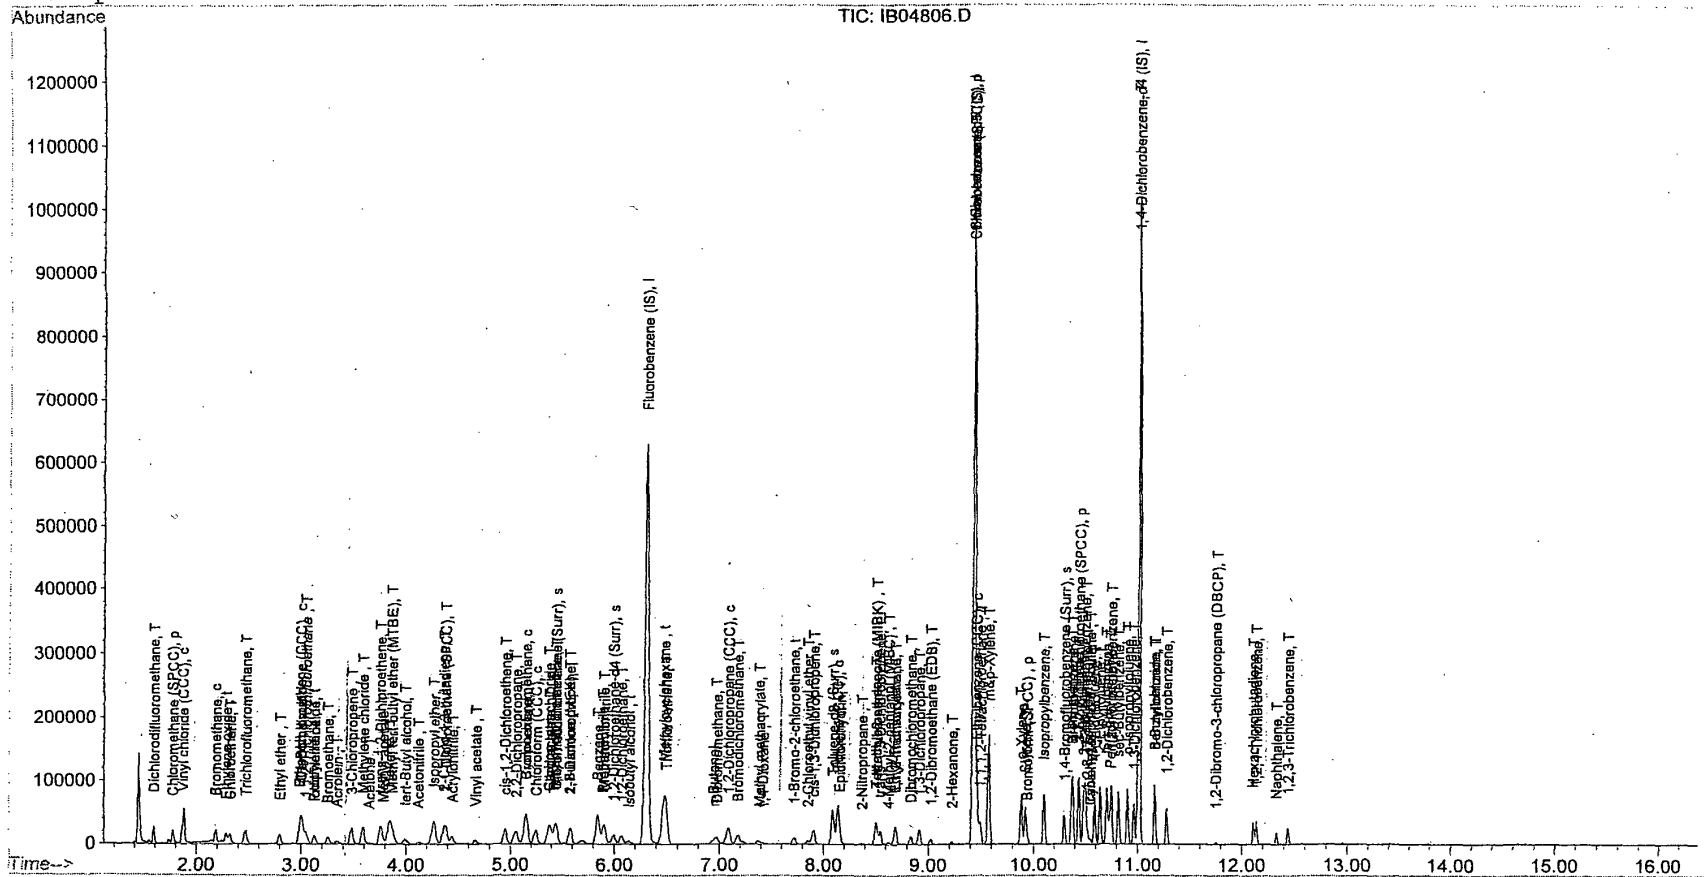

Quantitation Report (QT Reviewed) *K/A*

Data File : H:\MSI.I\I110408.B\IB04807.D
 Acq On : 4 Nov 2008 4:47 pm
 Sample : STD 2ppb
 Misc : 1,1, 2uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 5 11:34 19108

Vial: 7
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	706883	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.43	119	141692	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.01	152	189195	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.44	113	19298	2.0722	PPB	0.00
Spiked Amount	16.700		Recovery	=	12.40%	
50) 1,2-Dichloroethane-d4 (Sur)	6.00	67	11854	2.4695	PPB	0.00
Spiked Amount	16.700		Recovery	=	14.79%	
64) Toluene-d8 (Surr)	8.09	98	75512	1.8752	PPB	0.00
Spiked Amount	16.700		Recovery	=	11.26%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	25644	2.0294	PPB	0.00
Spiked Amount	16.700		Recovery	=	12.16%	
Target Compounds						
2) Dichlorodifluoromethane	1.59	85	29370	2.0152	PPB	99
3) Chloromethane (SPCC)	1.77	50	28164	1.4747	PPB	100
4) Vinyl chloride (CCC)	1.87	62	30065	1.7493	PPB	95
5) Bromomethane	2.19	94	17501	2.0792	PPB	98
6) Ethylene oxide	2.29	44	32010	28.1974	PPB	96
7) Chloroethane	2.32	64	22190	1.9853	PPB	100
8) Trichlorofluoromethane	2.47	101	32539	2.0398	PPB	100
9) Ethyl ether	2.80	59	17087	2.4008	PPB	97
10) Ethanol	2.98	45	2917	132.9094	PPB	74
11) 1,1-Dichloroethene (CCC)	2.99	96	19171	1.9005	PPB	96
12) Carbon disulfide	3.01	76	67454	1.8294	PPB	98
13) 1,1,2-Trichlorotrifluoroet	3.05	101	18992	1.9140	PPB	97
14) Propylene oxide	3.12	58	11554	11.5475	PPB	91
15) Iodomethane	3.12	142	14634	0.9103	PPB	94
16) Bromoethane	3.25	108	16655	1.9742	PPB	100
17) Acrolein	3.35	56	5583	8.8696	PPB	97
18) 3-Chloropropene	3.48	41	40856	1.9619	PPB	98
19) Methylene chloride	3.59	84	23298	2.1870	PPB	96
20) Acetone	3.65	58	993	2.6418	PPB	# 42
21) trans-1,2-Dichloroethene	3.76	96	22350	1.9855	PPB	96
22) Methyl acetate	3.78	74	4181	5.2035	PPB	90
23) Hexane	3.84	86	7258	1.7567	PPB	# 76
24) Methyl tert-butyl ether (M)	3.87	73	47230	2.3622	PPB	86
25) tert-Butyl alcohol	3.99	59	22279	121.9824	PPB	81
26) Acetonitrile	4.12	40	4221	18.3945	PPB	91
27) Isopropyl ether	4.27	45	84052	2.2330	PPB	96

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04807.D I81104W.M Thu Nov 06 11:53:32 2008 KMA Page 1

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04807.D
 Acq On : 4 Nov 2008 4:47 pm
 Sample : STD 2ppb
 Misc : 1,1, 2uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 5 11:34 19108

Vial: 7
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
28) 2-Chloro-1,3-butadiene	4.36	88	15701	1.6437	PPB	88
29) 1,1-Dichloroethane (SPCC)	4.38	63	45206	2.0884	PPB	100
30) Acrylonitrile	4.44	53	21021	13.4303	PPB	96
31) Vinyl acetate	4.66	43	25754	2.1731	PPB	97
32) cis-1,2-Dichloroethene	4.95	96	23980	2.0373	PPB	96
33) 2,2-Dichloropropane	5.05	77	32672	1.9270	PPB	95
34) Cyclohexane	5.15	56	39984	1.8749	PPB	96
35) Bromochloromethane	5.15	130	11011	2.1176	PPB	87
37) Chloroform (CCC)	5.25	83	39062	2.1930	PPB	99
38) Carbon tetrachloride	5.37	117	24514	1.9158	PPB	98
40) Ethyl acetate	5.38	43	53698	12.8915	PPB	98
41) Tetrahydrofuran	5.41	72	1457	2.3308	PPB	# 81
43) 1,1,1-Trichloroethane	5.44	97	31266	2.0303	PPB	98
44) 1,1-Dichloropropene	5.58	75	29687	1.9132	PPB	98
45) 2-Butanone (MEK)	5.58	43	4421	2.7538	PPB	85
46) Benzene	5.84	78	97242	1.9912	PPB	99
48) Propanenitrile	5.88	54	8136	15.1853	PPB	95
49) Methacrylonitrile	5.90	67	24705	11.5741	PPB	89
51) 1,2-Dichloroethane	6.07	62	24593	2.4812	PPB	97
52) Isobutyl alcohol	6.14	43	8817	100.8819	PPB	85
53) Methylcyclohexane	6.48	83	69959	3.4581	PPB	96
54) Trichloroethene	6.50	130	22367	1.9363	PPB	96
55) Dibromomethane	6.97	93	8303	2.2643	PPB	96
56) n-Butanol	6.93	56	9345	222.1908	PPB	88
57) 1,2-Dichloropropane (CCC)	7.08	63	22635	2.0941	PPB	90
58) Bromodichloromethane	7.18	83	25163	2.1245	PPB	98
59) 1,4-Dioxane	7.42	88	2421	149.9812	PPB	97
60) Methyl methacrylate	7.38	69	6762	1.8982	PPB	91
61) 1-Bromo-2-chloroethane	7.72	63	23973	2.2934	PPB	99
62) cis-1,3-Dichloropropene	7.90	75	30634	1.9685	PPB	97
63) 2-Chloroethyl vinyl ether	7.85	63	5885	1.8620	PPB	98
66) Toluene (CCC)	8.14	91	94402	2.0739	PPB	98
67) Epichlorohydrin	8.17	57	4596	14.3175	PPB	89
68) 2-Nitropropane	8.37	43	1856	1.6229	PPB	88
69) Tetrachloroethene	8.51	164	14672	1.8430	PPB	96
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	8976	2.4946	PPB	94
71) trans-1,3-Dichloropropene	8.55	75	23168	2.1946	PPB	97
72) 1,1,2-Trichloroethane	8.69	97	13151	2.5126	PPB	94
73) 4-Methyl-2-pentanol (MIBC)	8.62	45	6190	15.2947	PPB	75
74) Ethyl methacrylate	8.70	69	13071	1.9139	PPB	90
75) Dibromochloromethane	8.84	129	12818	2.2495	PPB	98

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist

TR04807.D I81104W.M

Thu Nov 06 11:53:32 2008

KMA

Page 2

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04807.D
 Acq On : 4 Nov 2008 4:47 pm
 Sample : STD 2ppb
 Misc : 1,1, 2uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 5 11:34 19108

Vial: 7
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
76) 1,3-Dichloropropane	8.91	76	26459	2.5256	PPB	94
77) 1,2-Dibromoethane (EDB)	9.02	107	11060	2.4174	PPB	97
78) 2-Hexanone	9.23	43	4987	2.3858	PPB	93
79) Chlorobenzene (SPCC)	9.44	112	56966	2.0691	PPB	92
80) 1-Chlorohexane	9.43	55	25033	2.2024	PPB	92
81) Ethylbenzene (CCC)	9.46	106	31113	1.9047	PPB	86
82) 1,1,1,2-Tetrachloroethane	9.49	131	17059	2.0880	PPB	98
83) m&p-Xylene	9.57	106	78015	3.8301	PPB	93
84) o-Xylene	9.88	106	35621	1.8663	PPB	93
85) Bromoform (SPCC)	9.94	173	5512	1.9874	PPB	98
86) Styrene	9.92	104	49102	1.7330	PPB	96
87) Isopropylbenzene	10.10	105	85488	1.9044	PPB	97
88) Bromobenzene	10.36	156	18384	2.0033	PPB #	88
89) n-Propylbenzene	10.38	120	23953	1.8003	PPB	89
90) 1,1,2,2-Tetrachloroethane	10.43	83	13256	2.5956	PPB	97
93) 2-Chlorotoluene	10.48	126	20612	1.8749	PPB #	86
94) Cyclohexanone	10.55	42	1005	25.0873	PPB	86
95) 1,2,3-Trichloropropane	10.52	110	4582	2.8402	PPB	99
96) trans-1,4-Dichloro-2-buten	10.54	53	2835	1.9816	PPB	75
97) 3-Ethyltoluene	10.43	105	88481	1.9011	PPB	99
98) 4-Chlorotoluene	10.59	126	20634	1.8880	PPB	89
99) 1,3,5-Trimethylbenzene	10.50	105	74766	1.9075	PPB	68
100) 2-Ethyltoluene	10.64	105	91366	1.9654	PPB	75
101) tert-Butylbenzene	10.70	91	42018	1.9674	PPB #	81
102) Pentachloroethane	10.73	167	10018	1.9141	PPB	92
103) 1,2,4-Trimethylbenzene	10.75	105	75670	1.9350	PPB	98
104) sec-Butylbenzene	10.81	105	91562	1.8853	PPB	98
105) p-Isopropyltoluene	10.90	119	77191	1.8228	PPB	97
106) 1,3-Dichlorobenzene	10.96	146	37514	1.9972	PPB	99
107) 1,4-Dichlorobenzene	11.01	146	40084	2.0502	PPB	94
108) Benzyl chloride	11.17	126	2300	0.9353	PPB #	1
109) n-Butylbenzene	11.16	134	16626	1.5499	PPB #	83
110) 1,2-Dichlorobenzene	11.28	146	30711	2.0553	PPB	97
112) 1,2-Dibromo-3-chloropropan	11.75	157	1189	3.6653	PPB	80
113) Hexachlorobutadiene	12.11	225	9320	1.6236	PPB	97
114) 1,2,4-Trichlorobenzene	12.14	180	15721	1.7582	PPB	98
115) Naphthalene	12.33	128	22287	1.8356	PPB	99
116) 1,2,3-Trichlorobenzene	12.43	180	11925	1.9719	PPB	98

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 TR04807.D I81104W.M Thu Nov 06 11:53:33 2008 KMA Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\I110408.B\IB04807.D
Acq On : 4 Nov 2008 4:47 pm
Sample : STD 2ppb
Misc : 1,1, 2uL/50mL 08MSV0802
MS Integration Params: VOA.P
Quant Time: Nov 4 17:03 19108

Vial: 7
Operator: kma
Inst : MSI
Multiplr: 1.00

Quant Results File: I81104W.RES

Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Wed Sep 24 14:27:06 2008
Response via : Initial Calibration

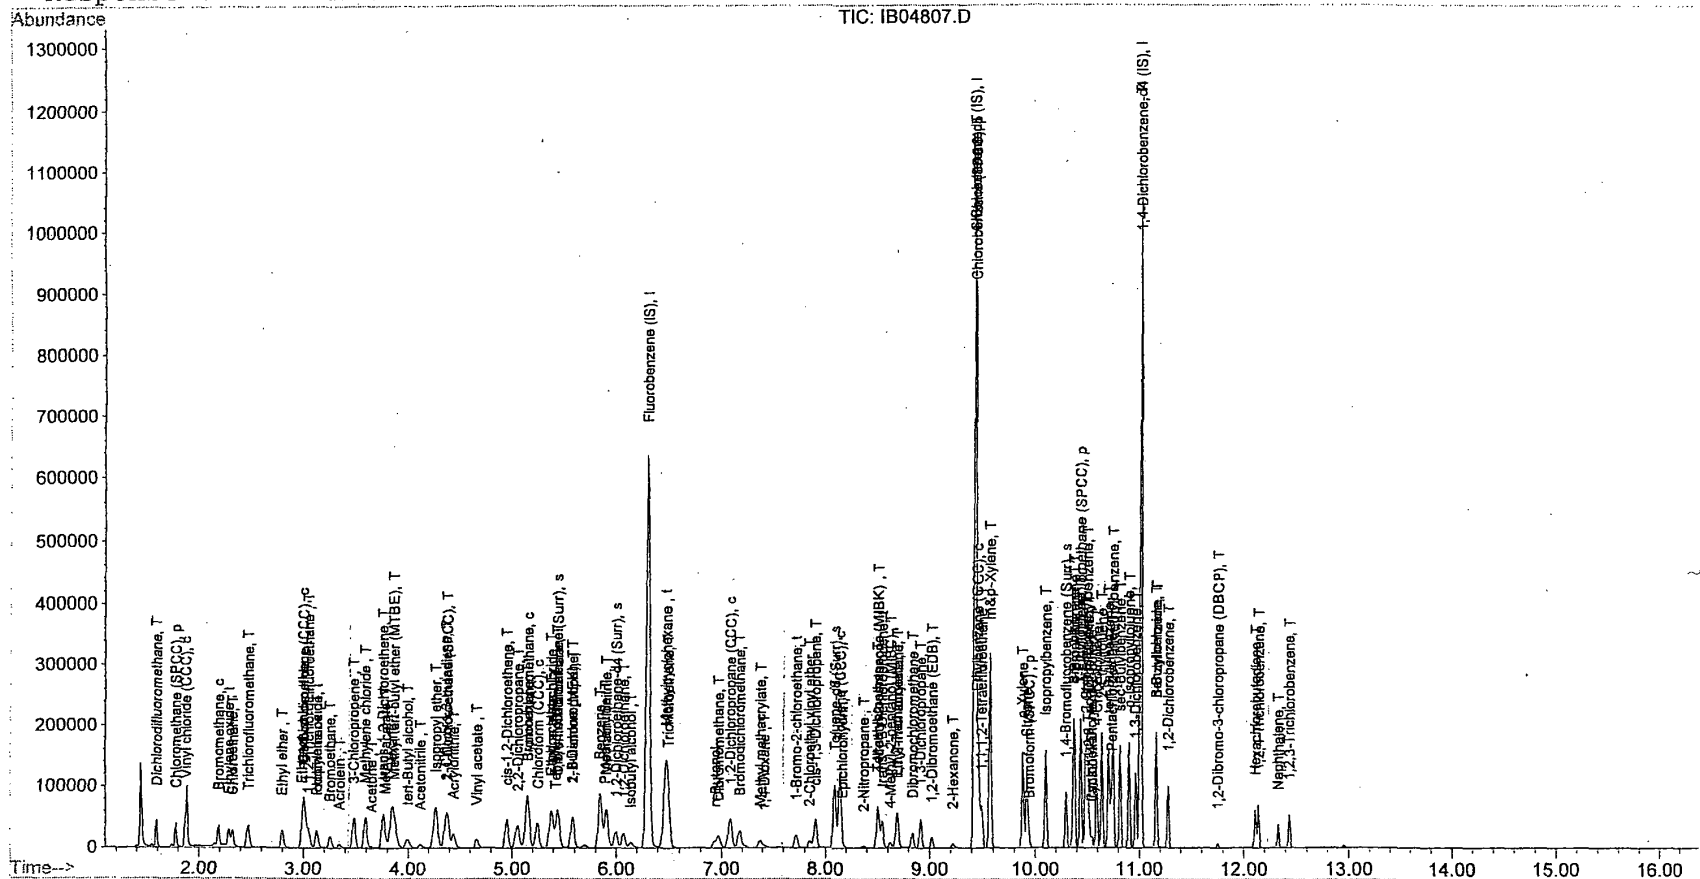

Quantitation Report (QT Reviewed) YA

NOV 06 20

Data File : H:\MSI.I\I110408.B\IB04808.D
 Acq On : 4 Nov 2008 5:14 pm
 Sample : STD 5ppb
 Misc : 1,1, 5uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 17:30 19108

Vial: 8
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Internal Standards	R.T.	QI on	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.30	96	697195	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.43	119	142180	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.00	152	191180	16.7000	PPB	0.00

System Monitoring Compounds

42) Dibromofluoromethane (Surr)	5.43	113	48817	5.3147	PPB	0.00
Spiked Amount	16.700		Recovery	=	31.80%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	27745	5.8603	PPB	0.00
Spiked Amount	16.700		Recovery	=	35.09%	
64) Toluene-d8 (Surr)	8.08	98	192128	4.8375	PPB	0.00
Spiked Amount	16.700		Recovery	=	28.98%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	64831	5.1131	PPB	0.00
Spiked Amount	16.700		Recovery	=	30.60%	

Target Compounds

Target Compounds	R.T.	QI on	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.59	85	77969	5.4242	PPB	100
3) Chloromethane (SPCC)	1.78	50	77076	4.0919	PPB	99
4) Vinyl chloride (CCC)	1.87	62	80591	4.7544	PPB	100
5) Bromomethane	2.19	94	40152	4.8364	PPB	99
6) Ethylene oxide	2.29	44	78132	69.7824	PPB	98
7) Chloroethane	2.32	64	55068	4.9953	PPB	99
8) Trichlorofluoromethane	2.47	101	84590	5.3763	PPB	99
9) Ethyl ether	2.80	59	42378	6.0371	PPB	96
10) Ethanol	2.97	45	7036	325.0411	PPB	74
11) 1,1-Dichloroethene (CCC)	2.99	96	50233	5.0490	PPB	95
12) Carbon disulfide	3.01	76	175937	4.8378	PPB	99
13) 1,1,2-Trichlorotrifluoroet	3.05	101	49466	5.0545	PPB	98
14) Propylene oxide	3.12	58	29918	30.3167	PPB	96
15) Iodomethane	3.13	142	54509	3.4377	PPB	96
16) Bromoethane	3.25	108	40562	4.8748	PPB	100
17) Acrolein	3.35	56	14232	22.9242	PPB	97
18) 3-Chloropropene	3.48	41	104961	5.1103	PPB	97
19) Methylene chloride	3.59	84	57692	5.4909	PPB	97
20) Acetone	3.65	58	2394	6.4575	PPB	# 66
21) trans-1,2-Dichloroethene	3.76	96	56683	5.1055	PPB	98
22) Methyl acetate	3.78	74	11346	14.3169	PPB	97
23) Hexane	3.84	86	19147	4.6986	PPB	# 76
24) Methyl tert-butyl ether (M	3.87	73	119432	6.0564	PPB	89
25) tert-Butyl alcohol	3.99	59	54166	300.6919	PPB	91
26) Acetonitrile	4.12	40	10714	47.3389	PPB	85
27) Isopropyl ether	4.26	45	213198	5.7427	PPB	97

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04808.D I81104W.M Thu Nov 06 11:53:38 2008 KMA Page 1

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04808.D
 Acq On : 4 Nov 2008 5:14 pm
 Sample : STD 5ppb
 Misc : 1,1, 5uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 17:30 19108

Vial: 8
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
28) 2-Chloro-1,3-butadiene	4.36	88	43577	4.6253	PPB	88
29) 1,1-Dichloroethane (SPCC)	4.39	63	111783	5.2358	PPB	99
30) Acrylonitrile	4.44	53	53850	34.8827	PPB	94
31) Vinyl acetate	4.66	43	68046	5.8216	PPB	98
32) cis-1,2-Dichloroethene	4.95	96	59367	5.1139	PPB	98
33) 2,2-Dichloropropane	5.05	77	84713	5.0658	PPB	97
34) Cyclohexane	5.15	56	107408	5.1064	PPB	96
35) Bromochloromethane	5.15	130	27416	5.3458	PPB	90
37) Chloroform (CCC)	5.24	83	97435	5.5462	PPB	99
38) Carbon tetrachloride	5.37	117	66499	5.2692	PPB	99
40) Ethyl acetate	5.38	43	136549	33.2375	PPB	99
41) Tetrahydrofuran	5.41	72	3582	5.8098	PPB #	43
43) 1,1,1-Trichloroethane	5.44	97	82367	5.4230	PPB	99
44) 1,1-Dichloropropene	5.58	75	78649	5.1390	PPB	98
45) 2-Butanone (MEK)	5.57	43	11185	7.0638	PPB	90
46) Benzene	5.84	78	243771	5.0611	PPB	99
48) Propanenitrile	5.88	54	20437	38.6744	PPB	95
49) Methacrylonitrile	5.90	67	65290	31.0130	PPB	94
51) 1,2-Dichloroethane	6.07	62	58722	6.0069	PPB	99
52) Isobutyl alcohol	6.14	43	23763	275.6683	PPB	94
53) Methylcyclohexane	6.47	83	185573	9.3004	PPB	96
54) Trichloroethene	6.50	130	55020	4.8291	PPB	96
55) Dibromomethane	6.97	93	20906	5.7804	PPB	95
56) n-Butanol	6.93	56	25631	543.5405	PPB	91
57) 1,2-Dichloropropane (CCC)	7.08	63	56636	5.3125	PPB	97
58) Bromodichloromethane	7.17	83	65325	5.5920	PPB	100
59) 1,4-Dioxane	7.42	88	6349	398.7865	PPB	92
60) Methyl methacrylate	7.37	69	18555	5.2811	PPB	93
61) 1-Bromo-2-chloroethane	7.72	63	58672	5.6908	PPB	99
62) cis-1,3-Dichloropropene	7.90	75	79522	5.1810	PPB	98
63) 2-Chloroethyl vinyl ether	7.85	63	15944	5.1146	PPB	97
66) Toluene (CCC)	8.14	91	238337	5.2180	PPB	98
67) Epichlorohydrin	8.16	57	12213	37.9155	PPB	83
68) 2-Nitropropane	8.36	43	4872	4.2454	PPB	87
69) Tetrachloroethene	8.50	164	38690	4.8432	PPB	98
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	23778	6.5855	PPB	96
71) trans-1,3-Dichloropropene	8.55	75	61672	5.8218	PPB	97
72) 1,1,2-Trichloroethane	8.69	97	32936	6.2710	PPB	95
73) 4-Methyl-2-pentanol (MIBC)	8.63	45	16967	41.7794	PPB	90
74) Ethyl methacrylate	8.69	69	36681	5.3525	PPB	91
75) Dibromochloromethane	8.83	129	34472	6.0289	PPB	99

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 TR04808.D I81104W.M Thu Nov 06 11:53:39 2008 KMA Page 2

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04808.D
 Acq On : 4 Nov 2008 5:14 pm
 Sample : STD 5ppb
 Misc : 1,1, 5uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 17:30 19108

Vial: 8
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
76) 1,3-Dichloropropane	8.91	76	65706	6.2504	PPB	96
77) 1,2-Dibromoethane (EDB)	9.02	107	28505	6.2091	PPB	99
78) 2-Hexanone	9.22	43	14508	6.9168	PPB	94
79) Chlorobenzene (SPCC)	9.44	112	142035	5.1411	PPB	96
80) 1-Chlorohexane	9.42	55	60203	5.1732	PPB	98
81) Ethylbenzene (CCC)	9.46	106	80673	4.9219	PPB	91
82) 1,1,1,2-Tetrachloroethane	9.49	131	44109	5.3803	PPB	98
83) m&p-Xylene	9.57	106	201702	9.8684	PPB	94
84) o-Xylene	9.88	106	93498	4.8818	PPB	93
85) Bromoform (SPCC)	9.94	173	14881	5.3470	PPB	100
86) Styrene	9.92	104	142468	5.0111	PPB	98
87) Isopropylbenzene	10.10	105	227628	5.0534	PPB	98
88) Bromobenzene	10.36	156	46808	5.0831	PPB #	90
89) n-Propylbenzene	10.37	120	63867	4.7837	PPB #	88
90) 1,1,2,2-Tetrachloroethane	10.43	83	33195	6.4776	PPB	99
93) 2-Chlorotoluene	10.48	126	53868	4.8490	PPB	89
94) Cyclohexanone	10.55	42	2634	65.0684	PPB	84
95) 1,2,3-Trichloropropane	10.52	110	11285	6.9225	PPB	96
96) trans-1,4-Dichloro-2-buten	10.54	53	7868	5.4424	PPB	80
97) 3-Ethyltoluene	10.43	105	234852	4.9936	PPB	98
98) 4-Chlorotoluene	10.58	126	53317	4.8278	PPB	90
99) 1,3,5-Trimethylbenzene	10.50	105	198444	5.0102	PPB	69
100) 2-Ethyltoluene	10.64	105	236466	5.0340	PPB	75
101) tert-Butylbenzene	10.70	91	109335	5.0663	PPB #	79
102) Pentachloroethane	10.73	167	26268	4.9667	PPB	94
103) 1,2,4-Trimethylbenzene	10.75	105	196961	4.9843	PPB	97
104) sec-Butylbenzene	10.82	105	239180	4.8736	PPB	98
105) p-Isopropyltoluene	10.90	119	205784	4.8090	PPB	97
106) 1,3-Dichlorobenzene	10.96	146	93665	4.9349	PPB	99
107) 1,4-Dichlorobenzene	11.02	146	98804	5.0012	PPB	97
108) Benzyl chloride	11.17	126	7949	3.1989	PPB #	42
109) n-Butylbenzene	11.16	134	46848	4.3218	PPB #	87
110) 1,2-Dichlorobenzene	11.27	146	78477	5.1975	PPB	99
112) 1,2-Dibromo-3-chloropropan	11.75	157	3374	6.2950	PPB	95
113) Hexachlorobutadiene	12.11	225	23638	4.0751	PPB	97
114) 1,2,4-Trichlorobenzene	12.14	180	41887	4.6358	PPB	100
115) Naphthalene	12.32	128	61249	4.9923	PPB	99
116) 1,2,3-Trichlorobenzene	12.43	180	29887	4.8906	PPB	97

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 TR04808.D I81104W.M Thu Nov 06 11:53:39 2008 KMA Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\I110408.B\IB04808.D
Acq On : 4 Nov 2008 5:14 pm
Sample : STD 5ppb
Misc : 1,1, 5uL/50mL 08MSV0802
MS Integration Params: VOA.P
Quant Time: Nov 4 17:30 19108

Vial: 8
Operator: kma
Inst : MSI
Multiplr: 1.00

Quant Results File: I81104W.RES

Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Wed Sep 24 14:27:06 2008
Response via : Initial Calibration

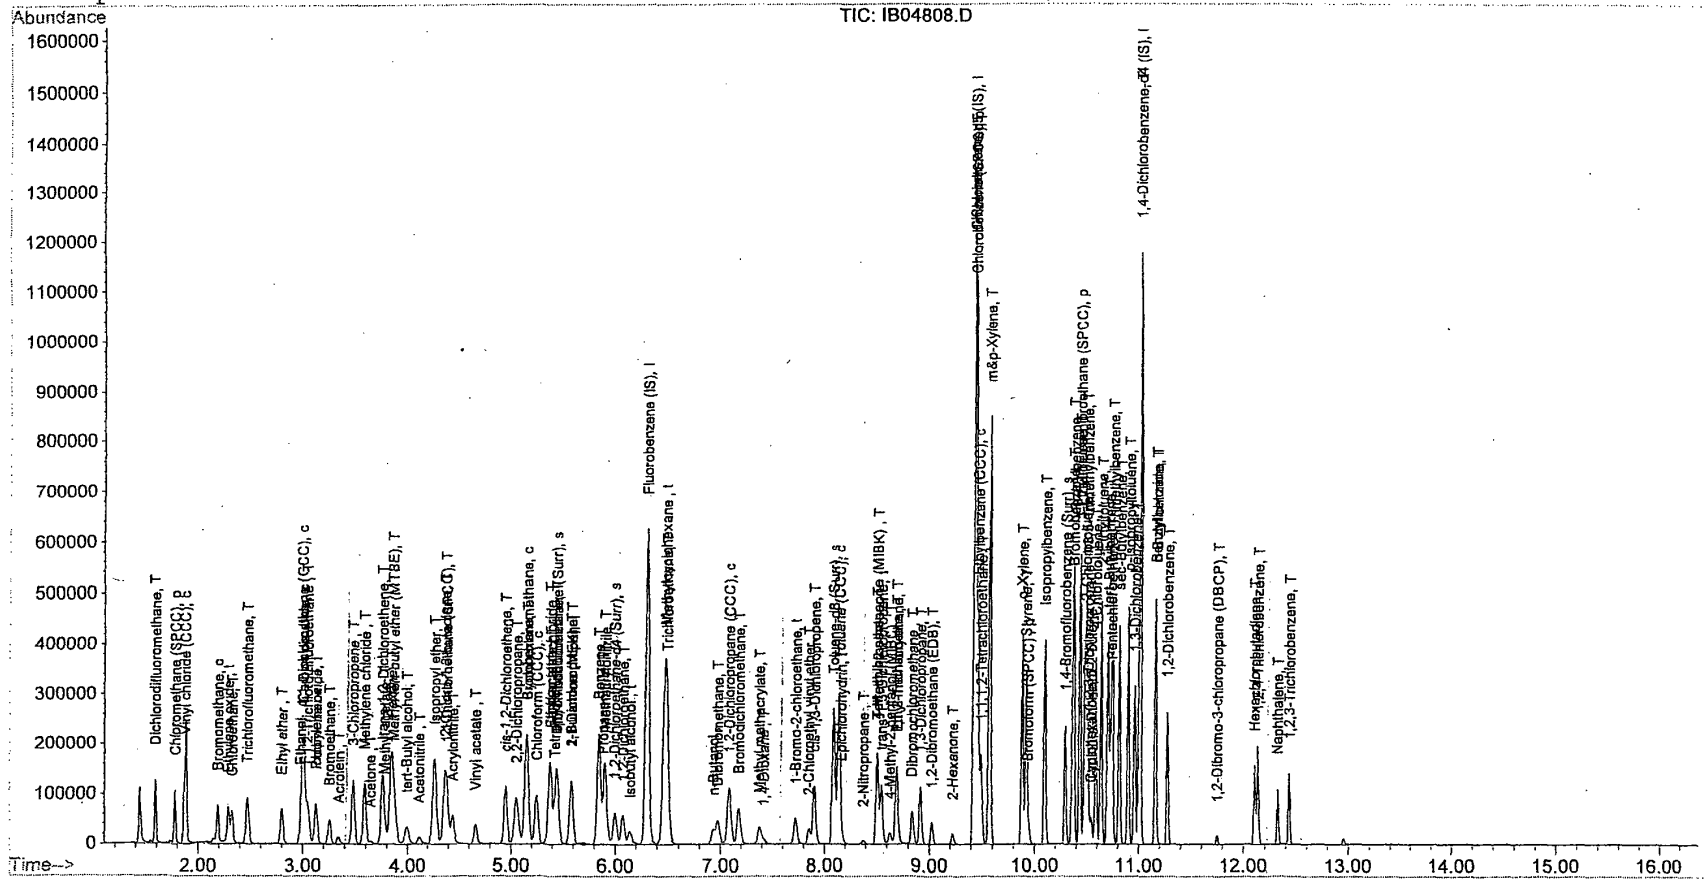

Data File : H:\MSI.I\I110408.B\IB04809.D
 Acq On : 4 Nov 2008 5:41 pm
 Sample : STD 10ppb
 Misc : 1,1, 10uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov. 4 17:57 19108

Vial: 9 *NOV 06 2008*
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.30	96	721459	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.43	119	150362	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.01	152	200217	16.7000	PPB	0.00

System Monitoring Compounds

42) Dibromofluoromethane (Surr)	5.43	113	105428	11.0920	PPB	0.00
Spiked Amount	16.700		Recovery	=	66.41%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	57645	11.7664	PPB	0.00
Spiked Amount	16.700		Recovery	=	70.48%	
64) Toluene-d8 (Surr)	8.09	98	416393	10.1317	PPB	0.00
Spiked Amount	16.700		Recovery	=	60.66%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	140714	10.4939	PPB	0.00
Spiked Amount	16.700		Recovery	=	62.81%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.59	85	159159	10.7001	PPB	100
3) Chloromethane (SPEC)	1.77	50	149780	7.6842	PPB	100
4) Vinyl chloride (CCC)	1.86	62	165997	9.4634	PPB	100
5) Bromomethane	2.19	94	75227	8.7566	PPB	100
6) Ethylene oxide	2.29	44	150925	130.2629	PPB	98
7) Chloroethane	2.32	64	114210	10.0117	PPB	100
8) Trichlorofluoromethane	2.47	101	171700	10.5458	PPB	99
9) Ethyl ether	2.79	59	88968	12.2480	PPB	97
10) Ethanol	2.98	45	15499	691.9246	PPB	75
11) 1,1-Dichloroethene (CCC)	2.99	96	104567	10.1568	PPB	94
12) Carbon disulfide	3.01	76	376486	10.0043	PPB	99
13) 1,1,2-Trichlorotrifluoroet	3.04	101	100786	9.9521	PPB	98
14) Propylene oxide	3.12	58	66492	65.1120	PPB	100
15) Iodomethane	3.13	142	145943	8.8946	PPB	96
16) Bromoethane	3.26	108	86243	10.0161	PPB	100
17) Acrolein	3.34	56	32147	50.0394	PPB	99
18) 3-Chloropropene	3.48	41	223077	10.4958	PPB	98
19) Methylene chloride	3.59	84	120654	11.0972	PPB	98
20) Acetone	3.65	58	5644	14.7120	PPB	92
21) trans-1,2-Dichloroethene	3.76	96	118621	10.3250	PPB	98
22) Methyl acetate	3.78	74	23395	28.5280	PPB	92
23) Hexane	3.84	86	40061	9.5001	PPB	# 78
24) Methyl tert-butyl ether (M	3.87	73	254856	12.4891	PPB	87
25) tert-Butyl alcohol	3.99	59	124762	669.2985	PPB	91
26) Acetonitrile	4.11	40	21998	93.9274	PPB	91
27) Isopropyl ether	4.26	45	454156	11.8218	PPB	98

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04809.D I81104W.M Thu Nov 06 11:53:45 2008 KMA Page 1

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04809.D
 Acq On : 4 Nov 2008 5:41 pm
 Sample : STD 10ppb
 Misc : 1,1, 10uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 17:57 19108

Vial: 9
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
28) 2-Chloro-1,3-butadiene	4.36	88	96122	9.8593	PPB	92
29) 1,1-Dichloroethane (SPCC)	4.38	63	235951	10.6800	PPB	100
30) Acrylonitrile	4.44	53	115684	72.4169	PPB	98
31) Vinyl acetate	4.66	43	153233	12.6687	PPB	99
32) cis-1,2-Dichloroethene	4.95	96	126385	10.5207	PPB	98
33) 2,2-Dichloropropane	5.05	77	178245	10.3004	PPB	98
34) Cyclohexane	5.14	56	221420	10.1728	PPB	96
35) Bromochloromethane	5.15	130	58914	11.1012	PPB	92
37) Chloroform (CCC)	5.24	83	202531	11.1408	PPB	99
38) Carbon tetrachloride	5.37	117	140768	10.7790	PPB	99
40) Ethyl acetate	5.37	43	299769	70.5130	PPB	99
41) Tetrahydrofuran	5.40	72	8466	13.2696	PPB	92
43) 1,1,1-Trichloroethane	5.44	97	171146	10.8893	PPB	99
44) 1,1-Dichloropropene	5.58	75	167075	10.5497	PPB	98
45) 2-Butanone (MEK)	5.57	43	24974	15.2417	PPB	86
46) Benzene	5.84	78	515826	10.3493	PPB	99
48) Propanenitrile	5.88	54	44256	80.9321	PPB	89
49) Methacrylonitrile	5.90	67	143917	66.0620	PPB	97
51) 1,2-Dichloroethane	6.07	62	125554	12.4114	PPB	99
52) Isobutyl alcohol	6.13	43	57100	640.1242	PPB	98
53) Methylcyclohexane	6.47	83	386384	18.7132	PPB	97
54) Trichloroethene	6.49	130	115997	9.8387	PPB	96
55) Dibromomethane	6.97	93	45616	12.1884	PPB	96
56) n-Butanol	6.93	56	69194	1445.5853	PPB	94
57) 1,2-Dichloropropane (CCC)	7.08	63	121883	11.0481	PPB	98
58) Bromodichloromethane	7.17	83	142891	11.8204	PPB	99
59) 1,4-Dioxane	7.41	88	14392	873.5724	PPB	89
60) Methyl methacrylate	7.37	69	43963	12.0920	PPB	95
61) 1-Bromo-2-chloroethane	7.72	63	128295	12.0253	PPB	100
62) cis-1,3-Dichloropropene	7.90	75	180434	11.3603	PPB	99
63) 2-Chloroethyl vinyl ether	7.85	63	37700	11.6869	PPB	98
66) Toluene (CCC)	8.14	91	510330	10.5648	PPB	99
67) Epichlorohydrin	8.17	57	27237	79.9566	PPB	82
68) 2-Nitropropane	8.37	43	11686	9.6290	PPB	91
69) Tetrachloroethene	8.51	164	82469	9.7618	PPB	99
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	55126	14.4369	PPB	97
71) trans-1,3-Dichloropropene	8.54	75	141804	12.6578	PPB	99
72) 1,1,2-Trichloroethane	8.68	97	70879	12.7609	PPB	97
73) 4-Methyl-2-pentanol (MIBC)	8.62	45	44134	102.7616	PPB	93
74) Ethyl methacrylate	8.70	69	92203	12.7223	PPB	97
75) Dibromochloromethane	8.84	129	78097	12.9155	PPB	98

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04809.D I81104W.M Thu Nov 06 11:53:45 2008 KMA Page 2

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04809.D
 Acq On : 4 Nov 2008 5:41 pm
 Sample : STD 10ppb
 Misc : 1,1, 10uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 17:57 19108

Vial: 9
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
76) 1,3-Dichloropropane	8.91	76	141794	12.7544	PPB	97
77) 1,2-Dibromoethane (EDB)	9.02	107	62973	12.9707	PPB	99
78) 2-Hexanone	9.22	43	33575	15.1360	PPB	96
79) Chlorobenzene (SPCC)	9.44	112	301718	10.3268	PPB	97
80) 1-Chlorohexane	9.43	55	120728	9.8279	PPB	99
81) Ethylbenzene (CCC)	9.46	106	176433	10.1785	PPB	90
82) 1,1,1,2-Tetrachloroethane	9.49	131	97467	11.2419	PPB	99
83) m&p-Xylene	9.57	106	443384	20.5125	PPB	96
84) o-Xylene	9.88	106	209583	10.3474	PPB	97
85) Bromoform (SPCC)	9.94	173	35428	12.0372	PPB	99
86) Styrene	9.92	104	329554	10.9608	PPB	98
87) Isopropylbenzene	10.09	105	490685	10.3005	PPB	98
88) Bromobenzene	10.36	156	102919	10.5683	PPB	93
89) n-Propylbenzene	10.37	120	139876	9.9067	PPB	91
90) 1,1,2,2-Tetrachloroethane	10.43	83	72098	13.3034	PPB	99
93) 2-Chlorotoluene	10.48	126	115663	9.9416	PPB	90
94) Cyclohexanone	10.54	42	5979	141.0342	PPB	86
95) 1,2,3-Trichloropropane	10.52	110	23716	13.8913	PPB	99
96) trans-1,4-Dichloro-2-buten	10.54	53	18880	12.4701	PPB	85
97) 3-Ethyltoluene	10.44	105	511029	10.3755	PPB	98
98) 4-Chlorotoluene	10.59	126	115693	10.0030	PPB	92
99) 1,3,5-Trimethylbenzene	10.50	105	427089	10.2962	PPB	68
100) 2-Ethyltoluene	10.64	105	514215	10.4528	PPB	76
101) tert-Butylbenzene	10.70	91	230934	10.2178	PPB	# 77
102) Pentachloroethane	10.73	167	60253	10.8784	PPB	96
103) 1,2,4-Trimethylbenzene	10.75	105	430850	10.4110	PPB	98
104) sec-Butylbenzene	10.81	105	513195	9.9851	PPB	98
105) p-Isopropyltoluene	10.90	119	448420	10.0063	PPB	98
106) 1,3-Dichlorobenzene	10.96	146	202595	10.1922	PPB	99
107) 1,4-Dichlorobenzene	11.01	146	212827	10.2865	PPB	99
108) Benzyl chloride	11.17	126	20213	7.7670	PPB	# 68
109) n-Butylbenzene	11.16	134	104425	9.1985	PPB	# 88
110) 1,2-Dichlorobenzene	11.27	146	171981	10.8760	PPB	99
112) 1,2-Dibromo-3-chloropropan	11.75	157	7920	11.3650	PPB	95
113) Hexachlorobutadiene	12.11	225	50025	8.2349	PPB	99
114) 1,2,4-Trichlorobenzene	12.14	180	93541	9.8853	PPB	100
115) Naphthalene	12.33	128	144804	11.2700	PPB	100
116) 1,2,3-Trichlorobenzene	12.43	180	66236	10.3495	PPB	99

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 I81104W.M Thu Nov 06 11:53:46 2008 KMA Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\I110408.B\IB04809.D
Acq On : 4 Nov 2008 5:41 pm
Sample : STD 10ppb
Misc : 1,1, 10uL/50mL 08MSV0802
MS Integration Params: VOA.P
Quant Time: Nov 4 17:57 19108

Vial: 9
Operator: kma
Inst : MSI
Multiplr: 1.00

Quant Results File: I81104W.RES

Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Wed Sep 24 14:27:06 2008
Response via : Initial Calibration

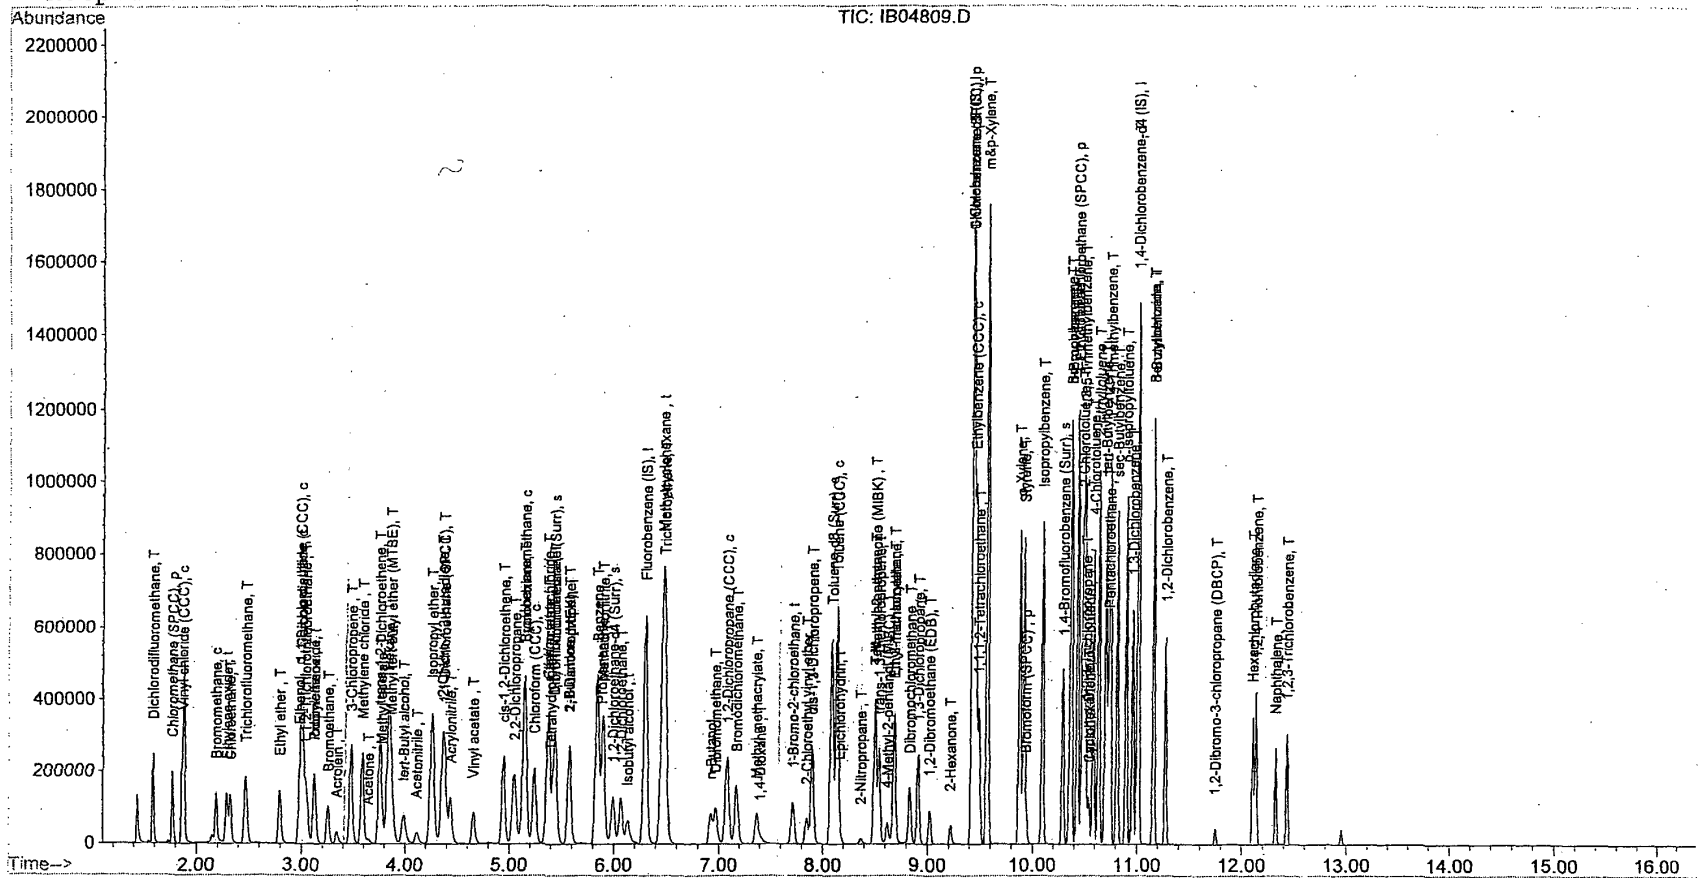

Quantitation Report

(QT Reviewed)

108/132

NOV 06 2008

Data File : H:\MSI.I\I110408.B\IB04810.D
 Acq On : 4 Nov 2008 6:08 pm
 Sample : STD 20ppb
 Misc : 1,1, 20uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 18:24 19108

Vial: 10
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.30	96	751704	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.43	119	159464	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.01	152	210863	16.7000	PPB	0.00

System Monitoring Compounds

42) Dibromofluoromethane (Surr)	5.43	113	221876	22.4041	PPB	0.00
Spiked Amount	16.700		Recovery	=	134.13%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	118682	23.2504	PPB	0.00
Spiked Amount	16.700		Recovery	=	139.22%	
64) Toluene-d8 (Surr)	8.08	98	884775	20.6621	PPB	0.00
Spiked Amount	16.700		Recovery	=	123.71%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	300944	21.1621	PPB	0.00
Spiked Amount	16.700		Recovery	=	126.71%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.59	85	325900	21.0284	PPB	99
3) Chloromethane (SPCC)	1.77	50	322672	15.8880	PPB	99
4) Vinyl chloride (CCC)	1.87	62	349002	19.0959	PPB	99
5) Bromomethane	2.19	94	162169	18.1173	PPB	99
6) Ethylene oxide	2.29	44	301529	249.7775	PPB	99
7) Chloroethane	2.32	64	237065	19.9450	PPB	99
8) Trichlorofluoromethane	2.47	101	353309	20.8271	PPB	99
9) Ethyl ether	2.80	59	187333	24.7521	PPB	97
10) Ethanol	2.97	45	32489	1392.0545	PPB	76
11) 1,1-Dichloroethene (CCC)	2.99	96	223281	20.8151	PPB	98
12) Carbon disulfide	3.01	76	806742	20.5749	PPB	100
13) 1,1,2-Trichlorotrifluoroet	3.04	101	210924	19.9897	PPB	97
14) Propylene oxide	3.12	58	139482	131.0916	PPB	99
15) Iodomethane	3.13	142	337908	19.7654	PPB	96
16) Bromoethane	3.25	108	181558	20.2375	PPB	99
17) Acrolein	3.34	56	68869	102.8869	PPB	99
18) 3-Chloropropene	3.48	41	471114	21.2741	PPB	98
19) Methylene chloride	3.59	84	250304	22.0956	PPB	98
20) Acetone	3.65	58	11469	28.6930	PPB	98
21) trans-1,2-Dichloroethene	3.76	96	250454	20.9229	PPB	99
22) Methyl acetate	3.78	74	50189	58.7384	PPB	95
23) Hexane	3.84	86	84773	19.2943	PPB	# 84
24) Methyl tert-butyl ether (M	3.87	73	530950	24.9721	PPB	86
25) tert-Butyl alcohol	3.98	59	267687	1378.2550	PPB	94
26) Acetonitrile	4.11	40	43370	177.7311	PPB	96
27) Isopropyl ether	4.26	45	953484	23.8207	PPB	99

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04810.D I81104W.M Thu Nov 06 11:53:52 2008 KMA Page 1

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04810.D
 Acq On : 4 Nov 2008 6:08 pm
 Sample : STD 20ppb
 Misc : 1,1, 20uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 18:24 19108

Vial: 10
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	Qion	Response	Conc	Unit	Qvalue
28) 2-Chloro-1,3-butadiene	4.36	88	209481	20.6220	PPB	94
29) 1,1-Dichloroethane (SPCC)	4.38	63	491809	21.3655	PPB	100
30) Acrylonitrile	4.43	53	238897	143.5299	PPB	98
31) Vinyl acetate	4.66	43	328475	26.0644	PPB	99
32) cis-1,2-Dichloroethene	4.94	96	265421	21.2056	PPB	98
33) 2,2-Dichloropropane	5.05	77	377467	20.9354	PPB	100
34) Cyclohexane	5.14	56	458202	20.2044	PPB	97
35) Bromochloromethane	5.15	130	125657	22.7249	PPB	96
37) Chloroform (CCC)	5.24	83	421695	22.2631	PPB	99
38) Carbon tetrachloride	5.37	117	293809	21.5925	PPB	100
40) Ethyl acetate	5.38	43	622307	140.4921	PPB	99
41) Tetrahydrofuran	5.40	72	18154	27.3097	PPB	96
43) 1,1,1-Trichloroethane	5.44	97	356710	21.7828	PPB	99
44) 1,1-Dichloropropene	5.58	75	348770	21.1364	PPB	99
45) 2-Butanone (MEK)	5.56	43	53710	31.4604	PPB	87
46) Benzene	5.84	78	1087419	20.9396	PPB	99
48) Propanenitrile	5.87	54	92074	161.6034	PPB	89
49) Methacrylonitrile	5.90	67	301582	132.8647	PPB	96
51) 1,2-Dichloroethane	6.07	62	253654	24.0655	PPB	99
52) Isobutyl alcohol	6.13	43	125945	1355.1079	PPB	98
53) Methylcyclohexane	6.47	83	806544	37.4905	PPB	98
54) Trichloroethene	6.50	130	246425	20.0604	PPB	97
55) Dibromomethane	6.97	93	96144	24.6557	PPB	96
56) n-Butanol	6.92	56	159793	4176.7689	PPB	97
57) 1,2-Dichloropropane (CCC)	7.08	63	254061	22.1029	PPB	99
58) Bromodichloromethane	7.17	83	298094	23.6671	PPB	100
59) 1,4-Dioxane	7.41	88	30477	1775.4759	PPB	91
60) Methyl methacrylate	7.37	69	98115	25.9006	PPB	98
61) 1-Bromo-2-chloroethane	7.72	63	269059	24.2046	PPB	99
62) cis-1,3-Dichloropropene	7.90	75	384886	23.2578	PPB	100
63) 2-Chloroethyl vinyl ether	7.85	63	81346	24.2025	PPB	99
66) Toluene (CCC)	8.14	91	1083275	21.1458	PPB	99
67) Epichlorohydrin	8.16	57	59591	164.9497	PPB	79
68) 2-Nitropropane	8.37	43	27845	21.6341	PPB	98
69) Tetrachloroethene	8.50	164	173296	19.3420	PPB	99
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	122050	30.1391	PPB	98
71) trans-1,3-Dichloropropene	8.55	75	304336	25.6152	PPB	100
72) 1,1,2-Trichloroethane	8.69	97	147224	24.9930	PPB	98
73) 4-Methyl-2-pentanol (MIBC)	8.62	45	105420	231.4495	PPB	95
74) Ethyl methacrylate	8.69	69	207496	26.9963	PPB	97
75) Dibromochloromethane	8.84	129	171533	26.7484	PPB	100

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04810.D I81104W.M Thu Nov 06 11:53:52 2008 KMA Page 2

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04810.D
 Acq On : 4 Nov 2008 6:08 pm
 Sample : STD 20ppb
 Misc : 1,1, 20uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 18:24 19108

Vial: 10
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W


Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
76) 1,3-Dichloropropane	8.91	76	294121	24.9461	PPB	99
77) 1,2-Dibromoethane (EDB)	9.02	107	131318	25.5040	PPB	99
78) 2-Hexanone	9.21	43	72324	30.7435	PPB	100
79) Chlorobenzene (SPCC)	9.44	112	643571	20.7699	PPB	98
80) 1-Chlorohexane	9.43	55	249565	19.5176	PPB	99
81) Ethylbenzene (CCC)	9.46	106	376393	20.4748	PPB	94
82) 1,1,1,2-Tetrachloroethane	9.49	131	207414	22.5577	PPB	99
83) m&p-Xylene	9.57	106	942627	41.1200	PPB	97
84) o-Xylene	9.88	106	445546	20.7417	PPB	97
85) Bromoform (SPCC)	9.94	173	77372	24.7879	PPB	99
86) Styrene	9.91	104	717918	22.5147	PPB	99
87) Isopropylbenzene	10.10	105	1047503	20.7342	PPB	99
88) Bromobenzene	10.36	156	217590	21.0681	PPB	94
89) n-Propylbenzene	10.38	120	296398	19.7942	PPB	91
90) 1,1,2,2-Tetrachloroethane	10.43	83	151779	26.4074	PPB	100
93) 2-Chlorotoluene	10.48	126	244401	19.9465	PPB	92
94) Cyclohexanone	10.55	42	11910	266.7523	PPB	94
95) 1,2,3-Trichloropropane	10.52	110	48884	27.1875	PPB	99
96) trans-1,4-Dichloro-2-buten	10.54	53	41281	25.8891	PPB	92
97) 3-Ethyltoluene	10.43	105	1074329	20.7111	PPB	98
98) 4-Chlorotoluene	10.59	126	246731	20.2556	PPB	96
99) 1,3,5-Trimethylbenzene	10.50	105	907102	20.7642	PPB	68
100) 2-Ethyltoluene	10.64	105	1078345	20.8135	PPB	76
101) tert-Butylbenzene	10.71	91	483359	20.3067	PPB	# 75
102) Pentachloroethane	10.73	167	134961	23.1363	PPB	97
103) 1,2,4-Trimethylbenzene	10.75	105	913077	20.9495	PPB	98
104) sec-Butylbenzene	10.81	105	1082241	19.9937	PPB	98
105) p-Isopropyltoluene	10.90	119	950279	20.1345	PPB	98
106) 1,3-Dichlorobenzene	10.96	146	431739	20.6235	PPB	99
107) 1,4-Dichlorobenzene	11.02	146	444790	20.4124	PPB	99
108) Benzyl chloride	11.17	126	51451	18.7724	PPB	92
109) n-Butylbenzene	11.16	134	225621	18.8709	PPB	# 87
110) 1,2-Dichlorobenzene	11.28	146	364803	21.9053	PPB	100
112) 1,2-Dibromo-3-chloropropan	11.75	157	18524	22.5401	PPB	99
113) Hexachlorobutadiene	12.11	225	106385	16.6285	PPB	99
114) 1,2,4-Trichlorobenzene	12.13	180	202339	20.3033	PPB	99
115) Naphthalene	12.32	128	321481	23.7574	PPB	100
116) 1,2,3-Trichlorobenzene	12.43	180	139818	20.7438	PPB	99

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04810.D I81104W.M Thu Nov 06 11:53:53 2008 KMA Page 3

Quantitation Report

Data File : C:\HPCHEM\1\DATA\I110408.B\IB04810.D Vial: 10
 Acq On : 4 Nov 2008 6:08 pm Operator: kma
 Sample : STD 20ppb Inst : MSI
 Misc : 1,1, 20uL/50mL 08MSV0802 Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Nov 4 18:24 19108 Quant Results File: I81104W.RES

Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration

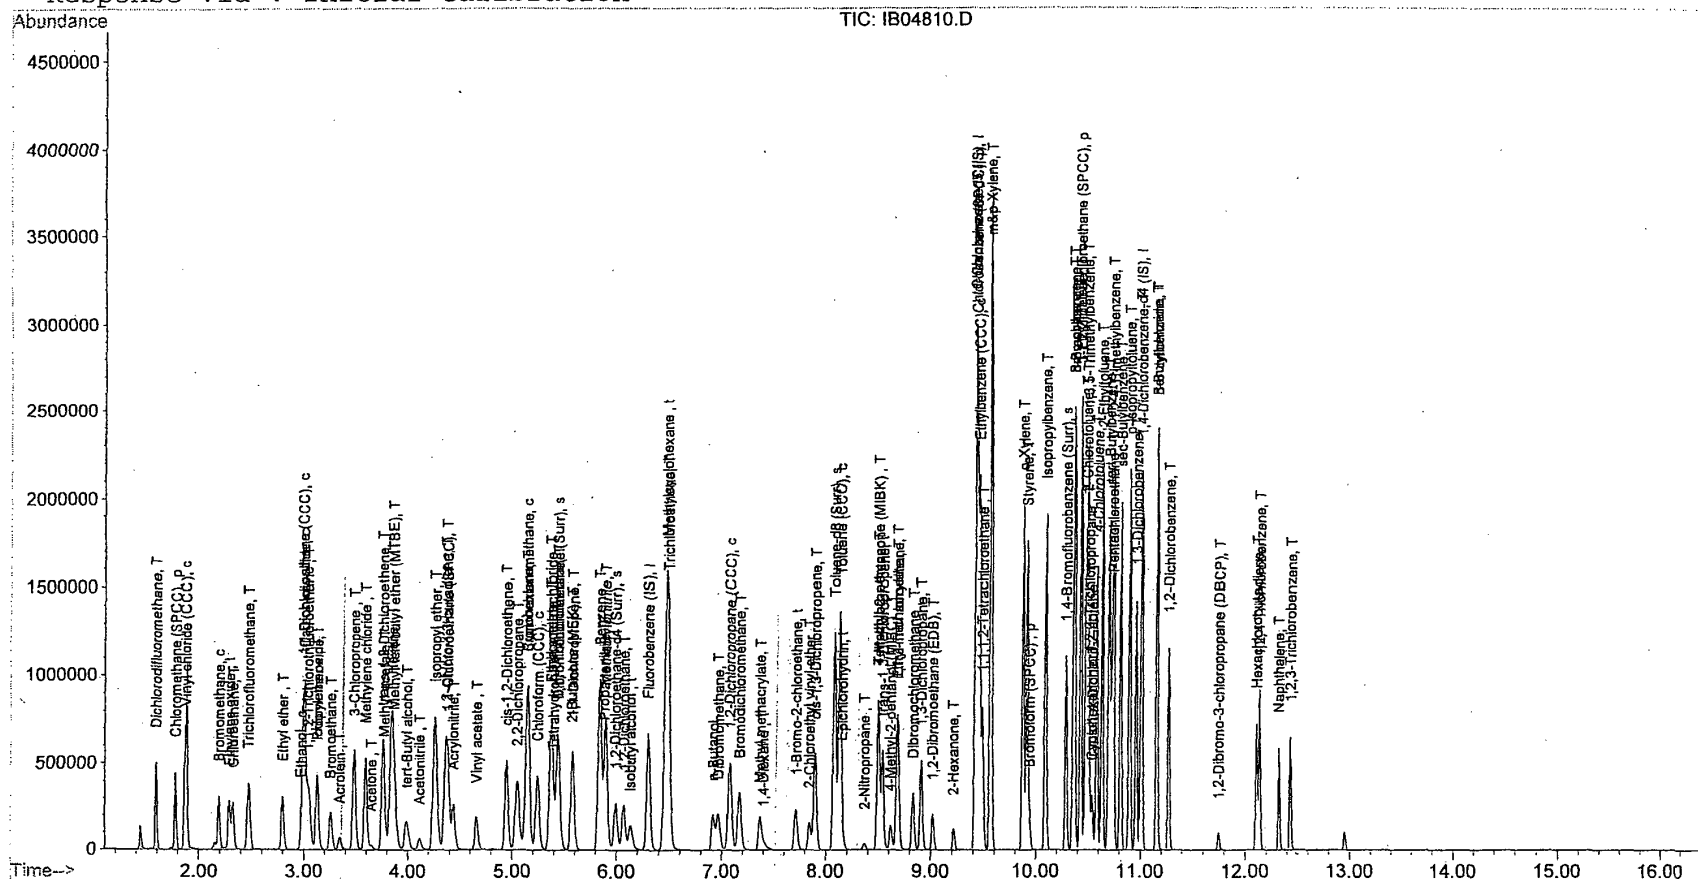

Data File : H:\MSI.I\I110408.B\IB04811.D
 Acq On : 4 Nov 2008 6:35 pm
 Sample : STD 50ppb
 Misc : 1,1, 50uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 18:52 19108

Vial: 11
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

NOV 06 2008

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	778154	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.43	119	175275	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.01	152	228642	16.7000	PPB	0.00

System Monitoring Compounds

42) Dibromofluoromethane (Surr)	5.43	113	581119	56.6845	PPB	0.00
Spiked Amount	16.700		Recovery	=	339.40%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	295705	55.9610	PPB	0.00
Spiked Amount	16.700		Recovery	=	335.09%	
64) Toluene-d8 (Surr)	8.08	98	2323636	52.4193	PPB	0.00
Spiked Amount	16.700		Recovery	=	313.89%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	795364	50.8841	PPB	0.00
Spiked Amount	16.700		Recovery	=	304.67%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.59	85	822185	51.2474	PPB	99
3) Chloromethane (SPCC)	1.77	50	853299	40.5874	PPB	100
4) Vinyl chloride (CCC)	1.87	62	911010	48.1524	PPB	100
5) Bromomethane	2.19	94	467991	50.5061	PPB	99
6) Ethylene oxide	2.29	44	525581	420.5767	PPB	98
7) Chloroethane	2.32	64	592958	48.1917	PPB	99
8) Trichlorofluoromethane	2.47	101	900504	51.2792	PPB	100
9) Ethyl ether	2.80	59	478189	61.0349	PPB	99
10) Ethanol	2.97	45	92180	3815.3809	PPB	76
11) 1,1-Dichloroethene (CCC)	2.99	96	590239	53.1541	PPB	100
12) Carbon disulfide	3.01	76	2153249	53.0491	PPB	99
13) 1,1,2-Trichlorotrifluoroet	3.04	101	544428	49.8427	PPB	98
14) Propylene oxide	3.12	58	358861	325.8098	PPB	100
15) Iodomethane	3.12	142	903623	51.0595	PPB	98
16) Bromoethane	3.25	108	471358	50.7543	PPB	99
17) Acrolein	3.34	56	184651	266.4828	PPB	99
18) 3-Chloropropene	3.48	41	1204278	52.5331	PPB	97
19) Methylene chloride	3.59	84	644807	54.9855	PPB	99
20) Acetone	3.64	58	30292	73.2082	PPB	93
21) trans-1,2-Dichloroethene	3.75	96	652644	52.6687	PPB	99
22) Methyl acetate	3.78	74	130771	147.8449	PPB	93
23) Hexane	3.84	86	222411	48.9000	PPB	# 89
24) Methyl tert-butyl ether (M	3.87	73	1373079	62.3847	PPB	84
25) tert-Butyl alcohol	3.98	59	746267	3711.7426	PPB	95
26) Acetonitrile	4.11	40	113124	447.8267	PPB	99
27) Isopropyl ether	4.26	45	2409892	58.1595	PPB	99

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04811.D I81104W.M Thu Nov 06 11:54:00 2008 KMA Page 1

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04811.D Vial: 11
 Acq On : 4 Nov 2008 6:35 pm Operator: kma
 Sample : STD 50ppb Inst : MSI
 Misc : 1,1, 50uL/50mL 08MSV0802 Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Nov 4 18:52 19108 Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
28) 2-Chloro-1,3-butadiene	4.36	88	554565	52.7377	PPB	97
29) 1,1-Dichloroethane (SPCC)	4.38	63	1249885	52.4527	PPB	100
30) Acrylonitrile	4.43	53	620586	360.1762	PPB	98
31) Vinyl acetate	4.65	43	856686	65.6672	PPB	100
32) cis-1,2-Dichloroethene	4.94	96	699311	53.9717	PPB	99
33) 2,2-Dichloropropane	5.05	77	961228	51.5002	PPB	98
34) Cyclohexane	5.14	56	1186636	50.5460	PPB	99
35) Bromochloromethane	5.15	130	329254	57.5211	PPB	98
37) Chloroform (CCC)	5.24	83	1085607	55.3658	PPB	99
38) Carbon tetrachloride	5.37	117	753617	53.5021	PPB	100
40) Ethyl acetate	5.37	43	1585991	345.8831	PPB	100
41) Tetrahydrofuran	5.40	72	48572	70.5849	PPB	96
43) 1,1,1-Trichloroethane	5.44	97	928979	54.8005	PPB	99
44) 1,1-Dichloropropene	5.58	75	904889	52.9748	PPB	98
45) 2-Butanone (MEK)	5.56	43	141321	79.9645	PPB	86
46) Benzene	5.84	78	2797839	52.0445	PPB	99
48) Propanenitrile	5.87	54	241989	410.2895	PPB	90
49) Methacrylonitrile	5.90	67	795472	338.5404	PPB	99
51) 1,2-Dichloroethane	6.07	62	641507	58.7945	PPB	100
52) Isobutyl alcohol	6.13	43	364961	3793.3308	PPB	99
53) Methylcyclohexane	6.47	83	2132511	95.7560	PPB	100
54) Trichloroethene	6.49	130	654851	51.4967	PPB	98
55) Dibromomethane	6.97	93	250063	61.9478	PPB	98
56) n-Butanol	6.91	56	484883	-16.7000	PPB	98
57) 1,2-Dichloropropane (CCC)	7.08	63	655307	55.0728	PPB	99
58) Bromodichloromethane	7.17	83	781032	59.9020	PPB	99
59) 1,4-Dioxane	7.41	88	86850	4887.5780	PPB	93
60) Methyl methacrylate	7.37	69	271336	69.1932	PPB	99
61) 1-Bromo-2-chloroethane	7.72	63	697942	60.6528	PPB	99
62) cis-1,3-Dichloropropene	7.90	75	1012242	59.0883	PPB	99
63) 2-Chloroethyl vinyl ether	7.85	63	213420	61.3394	PPB	98
66) Toluene (GCC)	8.14	91	2831134	50.2792	PPB	99
67) Epichlorohydrin	8.16	57	159650	402.0521	PPB	77
68) 2-Nitropropane	8.37	43	82377	58.2291	PPB	99
69) Tetrachloroethene	8.50	164	472477	47.9773	PPB	99
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	328469	73.7954	PPB	98
71) trans-1,3-Dichloropropene	8.54	75	796600	60.9996	PPB	99
72) 1,1,2-Trichloroethane	8.68	97	387508	59.8499	PPB	99
73) 4-Methyl-2-pentanol (MIBC)	8.62	45	348093	695.2982	PPB	99
74) Ethyl methacrylate	8.69	69	575290	68.0964	PPB	99
75) Dibromochloromethane	8.84	129	459154	65.1406	PPB	99

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04811.D I81104W.M Thu Nov 06 11:54:00 2008 KMA Page 2

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04811.D
 Acq On : 4 Nov 2008 6:35 pm
 Sample : STD 50ppb
 Misc : 1,1, 50uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 18:52 19108

Vial: 11
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
76) 1,3-Dichloropropane	8.91	76	759730	58.6244	PPB	100
77) 1,2-Dibromoethane (EDB)	9.02	107	355370	62.7925	PPB	99
78) 2-Hexanone	9.21	43	208635	80.6866	PPB	99
79) Chlorobenzene (SPCC)	9.44	112	1760107	51.6797	PPB	99
80) 1-Chlorohexane	9.43	55	633495	48.4188	PPB	99
81) Ethylbenzene (CCC)	9.46	106	1017058	50.3347	PPB	96
82) 1,1,1,2-Tetrachloroethane	9.49	131	560420	55.4514	PPB	100
83) m&p-Xylene	9.57	106	2597490	103.0884	PPB	98
84) o-Xylene	9.88	106	1212725	51.3639	PPB	99
85) Bromoform (SPCC)	9.94	173	220127	64.1611	PPB	99
86) Styrene	9.92	104	1970865	56.2329	PPB	99
87) Isopropylbenzene	10.10	105	2796034	50.3519	PPB	100
88) Bromobenzene	10.36	156	604861	53.2826	PPB	98
89) n-Propylbenzene	10.38	120	828097	50.3138	PPB	99
90) 1,1,2,2-Tetrachloroethane	10.43	83	413567	65.4641	PPB	100
93) 2-Chlorotoluene	10.48	126	672974	50.6530	PPB	98
94) Cyclohexanone	10.55	42	37110	766.5346	PPB	# 84
95) 1,2,3-Trichloropropane	10.52	110	132038	67.7245	PPB	100
96) trans-1,4-Dichloro-2-buten	10.54	53	118310	68.4279	PPB	96
97) 3-Ethyltoluene	10.43	105	2919070	51.8984	PPB	100
98) 4-Chlorotoluene	10.59	126	667544	50.5413	PPB	99
99) 1,3,5-Trimethylbenzene	10.50	105	2422645	51.1439	PPB	66
100) 2-Ethyltoluene	10.64	105	2874655	51.1701	PPB	77
101) tert-Butylbenzene	10.70	91	1272830	49.3157	PPB	# 72
102) Pentachloroethane	10.73	167	377156	59.6282	PPB	99
103) 1,2,4-Trimethylbenzene	10.75	105	2447612	51.7909	PPB	100
104) sec-Butylbenzene	10.81	105	2918819	49.7303	PPB	99
105) p-Isopropyltoluene	10.90	119	2582466	50.4624	PPB	100
106) 1,3-Dichlorobenzene	10.96	146	1180005	51.9839	PPB	100
107) 1,4-Dichlorobenzene	11.01	146	1231750	52.1323	PPB	99
108) Benzyl chloride	11.17	126	165445	55.6703	PPB	89
109) n-Butylbenzene	11.16	134	627989	48.4406	PPB	# 89
110) 1,2-Dichlorobenzene	11.28	146	983263	54.4508	PPB	100
112) 1,2-Dibromo-3-chloropropan	11.75	157	58584	61.5043	PPB	98
113) Hexachlorobutadiene	12.11	225	300014	43.2474	PPB	100
114) 1,2,4-Trichlorobenzene	12.14	180	555790	51.4330	PPB	100
115) Naphthalene	12.32	128	893299	60.8814	PPB	100
116) 1,2,3-Trichlorobenzene	12.43	180	382719	52.3661	PPB	99

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04811.D I81104W.M Thu Nov 06 11:54:01 2008 KMA Page 3

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04812.D
 Acq On : 4 Nov 2008 7:02 pm
 Sample : STD 100ppb
 Misc : 1,1, 100uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 19:19 19108

Vial: 12
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

KA
 NOV 06 2008

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	823197	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	189191	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.01	152	251636	16.7000	PPB	0.00

System Monitoring Compounds

42) Dibromofluoromethane (Surr)	5.43	113	1237095	114.0680	PPB	0.00
Spiked Amount	16.700		Recovery	=	683.05%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	611553	109.4013	PPB	0.00
Spiked Amount	16.700		Recovery	=	655.09%	
64) Toluene-d8 (Surr)	8.09	98	4894875	104.3822	PPB	0.00
Spiked Amount	16.700		Recovery	=	625.03%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	1695791	100.5097	PPB	0.00
Spiked Amount	16.700		Recovery	=	601.86%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.59	85	1578481	93.0044	PPB	99
3) Chloromethane (SPCC)	1.77	50	1810359	81.3986	PPB	99
4) Vinyl chloride (CCC)	1.86	62	1836157	91.7415	PPB	100
5) Bromomethane	2.19	94	1093845	111.5897	PPB	99
6) Ethylene oxide	2.28	44	577077	436.5170	PPB	97
7) Chloroethane	2.31	64	1011546	77.7134	PPB	98
8) Trichlorofluoromethane	2.46	101	1746461	94.0104	PPB	100
9) Ethyl ether	2.79	59	979589	118.1910	PPB	100
10) Ethanol	2.97	45	181924	7117.9179	PPB	77
11) 1,1-Dichloroethene (CCC)	2.99	96	1233598	105.0132	PPB	96
12) Carbon disulfide	3.01	76	4467581	104.0442	PPB	98
13) 1,1,2-Trichlorotrifluoroet	3.04	101	1081134	93.5627	PPB	99
14) Propylene oxide	3.12	58	725917	622.9979	PPB	97
15) Iodomethane	3.13	142	1906322	101.8233	PPB	99
16) Bromoethane	3.26	108	1008628	102.6631	PPB	100
17) Acrolein	3.33	56	390964	533.3545	PPB	99
18) 3-Chloropropene	3.47	41	2442551	100.7190	PPB	98
19) Methylene chloride	3.59	84	1344405	108.3703	PPB	97
20) Acetone	3.64	58	64737	147.8925	PPB	98
21) trans-1,2-Dichloroethene	3.75	96	1394386	106.3704	PPB	97
22) Methyl acetate	3.77	74	271117	289.7434	PPB	99
23) Hexane	3.84	86	434815	90.3689	PPB	# 92
24) Methyl tert-butyl ether (M	3.86	73	2804971	120.4683	PPB	79
25) tert-Butyl alcohol	3.99	59	1509739	7098.1842	PPB	96
26) Acetonitrile	4.11	40	230452	862.3776	PPB	98
27) Isopropyl ether	4.26	45	4828208	110.1466	PPB	99

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04812.D I81104W.M Thu Nov 06 11:54:06 2008 KMA Page 1

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04812.D
 Acq On : 4 Nov 2008 7:02 pm
 Sample : STD 100ppb
 Misc : 1,1, 100uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 19:19 19108

Vial: 12
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
28) 2-Chloro-1,3-butadiene	4.36	88	1170247	105.1980	PPB	98
29) 1,1-Dichloroethane (SPCC)	4.38	63	2580267	102.3585	PPB	99
30) Acrylonitrile	4.44	53	1282158	703.4226	PPB	99
31) Vinyl acetate	4.65	43	1746274	126.5322	PPB	99
32) cis-1,2-Dichloroethene	4.95	96	1481554	108.0874	PPB	97
33) 2,2-Dichloropropane	5.05	77	1976216	100.0873	PPB	97
34) Cyclohexane	5.14	56	2314919	93.2110	PPB	99
35) Bromochloromethane	5.15	130	707645	116.8621	PPB	96
37) Chloroform (CCC)	5.25	83	2269146	109.3940	PPB	99
38) Carbon tetrachloride	5.37	117	1548898	103.9452	PPB	100
40) Ethyl acetate	5.37	43	3154887	650.3905	PPB	99
41) Tetrahydrofuran	5.40	72	100555	138.1310	PPB	91
43) 1,1,1-Trichloroethane	5.44	97	1910198	106.5170	PPB	98
44) 1,1-Dichloropropene	5.57	75	1862996	103.0974	PPB	97
45) 2-Butanone (MEK)	5.56	43	291377	155.8503	PPB	86
46) Benzene	5.84	78	5816419	102.2750	PPB	99
48) Propanenitrile	5.87	54	495630	794.3541	PPB	90
49) Methacrylonitrile	5.90	67	1637640	658.8186	PPB	97
51) 1,2-Dichloroethane	6.07	62	1306281	113.1705	PPB	99
52) Isobutyl alcohol	6.13	43	753076	7399.0308	PPB	99
53) Methylcyclohexane	6.47	83	4222040	179.2086	PPB	98
54) Trichloroethene	6.49	130	1421182	105.6449	PPB	99
55) Dibromomethane	6.97	93	525857	123.1418	PPB	98
56) n-Butanol	6.92	56	995296	-16.7000	PPB	98
57) 1,2-Dichloropropane (CCC)	7.08	63	1373978	109.1525	PPB	98
58) Bromodichloromethane	7.17	83	1667565	120.8975	PPB	99
59) 1,4-Dioxane	7.40	88	172257	9163.5242	PPB	93
60) Methyl methacrylate	7.37	69	571218	137.6954	PPB	98
61) 1-Bromo-2-chloroethane	7.71	63	1464845	120.3331	PPB	99
62) cis-1,3-Dichloropropene	7.90	75	2125076	117.2610	PPB	97
63) 2-Chloroethyl vinyl ether	7.85	63	434615	118.0785	PPB	97
66) Toluene (CCC)	8.13	91	5936320	97.6709	PPB	100
67) Epichlorohydrin	8.16	57	321552	750.2122	PPB	77
68) 2-Nitropropane	8.37	43	182321	119.3962	PPB	98
69) Tetrachloroethene	8.51	164	1015125	95.4980	PPB	99
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	664329	138.2731	PPB	98
71) trans-1,3-Dichloropropene	8.54	75	1673949	118.7541	PPB	98
72) 1,1,2-Trichloroethane	8.68	97	825284	118.0880	PPB	99
73) 4-Methyl-2-pentanol (MIBC)	8.62	45	748129	1384.4326	PPB	99
74) Ethyl methacrylate	8.69	69	1212330	132.9468	PPB	98
75) Dibromochloromethane	8.83	129	990043	130.1268	PPB	99

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04812.D I81104W.M Thu Nov 06 11:54:06 2008 KMA Page 2

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04812.D
 Acq On : 4 Nov 2008 7:02 pm
 Sample : STD 100ppb
 Misc : 1,1, 100uL/50mL 08MSV0802
 MS Integration Params: VOA.P
 Quant Time: Nov 4 19:19 19108

Vial: 12
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W


Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
76) 1,3-Dichloropropane	8.91	76	1592477	113.8443	PPB	98
77) 1,2-Dibromoethane (EDB)	9.02	107	745925	122.1073	PPB	100
78) 2-Hexanone	9.22	43	434795	155.7823	PPB	98
79) Chlorobenzene (SPCC)	9.44	112	3770588	102.5675	PPB	97
80) 1-Chlorohexane	9.42	55	1248670	103.6983	PPB	98
81) Ethylbenzene (CCC)	9.46	106	2200868	100.9101	PPB	98
82) 1,1,1,2-Tetrachloroethane	9.49	131	1212805	111.1755	PPB	99
83) m&p-Xylene	9.57	106	5455438	200.5881	PPB	92
84) o-Xylene	9.88	106	2608743	102.3637	PPB	97
85) Bromoform (SPCC)	9.94	173	481135	129.9227	PPB	99
86) Styrene	9.92	104	4230347	111.8224	PPB	98
87) Isopropylbenzene	10.09	105	5867905	97.8986	PPB	99
88) Bromobenzene	10.36	156	1342437	109.5578	PPB	97
89) n-Propylbenzene	10.37	120	1804211	101.5576	PPB	91
90) 1,1,2,2-Tetrachloroethane	10.43	83	875987	128.4619	PPB	100
93) 2-Chlorotoluene	10.48	126	1465371	100.2162	PPB	98
94) Cyclohexanone	10.54	42	75597	1418.8244	PPB #	84
95) 1,2,3-Trichloropropane	10.52	110	278179	129.6447	PPB	100
96) trans-1,4-Dichloro-2-buten	10.54	53	249010	130.8615	PPB	97
97) 3-Ethyltoluene	10.43	105	6084671	98.2947	PPB	98
98) 4-Chlorotoluene	10.59	126	1449962	99.7484	PPB	95
99) 1,3,5-Trimethylbenzene	10.50	105	5108557	97.9908	PPB	63
100) 2-Ethyltoluene	10.64	105	6014152	97.2721	PPB	78
101) tert-Butylbenzene	10.70	91	2659646	93.6314	PPB #	68
102) Pentachloroethane	10.73	167	854212	122.7099	PPB	99
103) 1,2,4-Trimethylbenzene	10.75	105	5132327	98.6753	PPB	98
104) sec-Butylbenzene	10.82	105	6035226	93.4310	PPB	99
105) p-Isopropyltoluene	10.90	119	5422845	96.2817	PPB	99
106) 1,3-Dichlorobenzene	10.96	146	2580243	103.2830	PPB	99
107) 1,4-Dichlorobenzene	11.02	146	2667718	102.5905	PPB	99
108) Benzyl chloride	11.16	126	393605	120.3410	PPB #	76
109) n-Butylbenzene	11.16	134	1382034	96.8633	PPB	97
110) 1,2-Dichlorobenzene	11.27	146	2152363	108.3013	PPB	99
112) 1,2-Dibromo-3-chloropropan	11.75	157	126855	118.8698	PPB	97
113) Hexachlorobutadiene	12.11	225	654713	85.7536	PPB	100
114) 1,2,4-Trichlorobenzene	12.14	180	1204649	101.2920	PPB	99
115) Naphthalene	12.33	128	1864167	115.4398	PPB	100
116) 1,2,3-Trichlorobenzene	12.44	180	819206	101.8465	PPB	100

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04812.D I81104W.M Thu Nov 06 11:54:07 2008 KMA Page 3

Quantitation Report

Data File : C:\HPCHEM\1\DATA\I110408.B\IB04812.D Vial: 12
 Acq On : 4 Nov 2008 7:02 pm Operator: kma
 Sample : STD 100ppb Inst : MSI
 Misc : 1,1, 100uL/50mL 08MSV0802 Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Nov 4 19:19 19108 Quant Results File: I81104W.RES

Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Sep 24 14:27:06 2008
 Response via : Initial Calibration

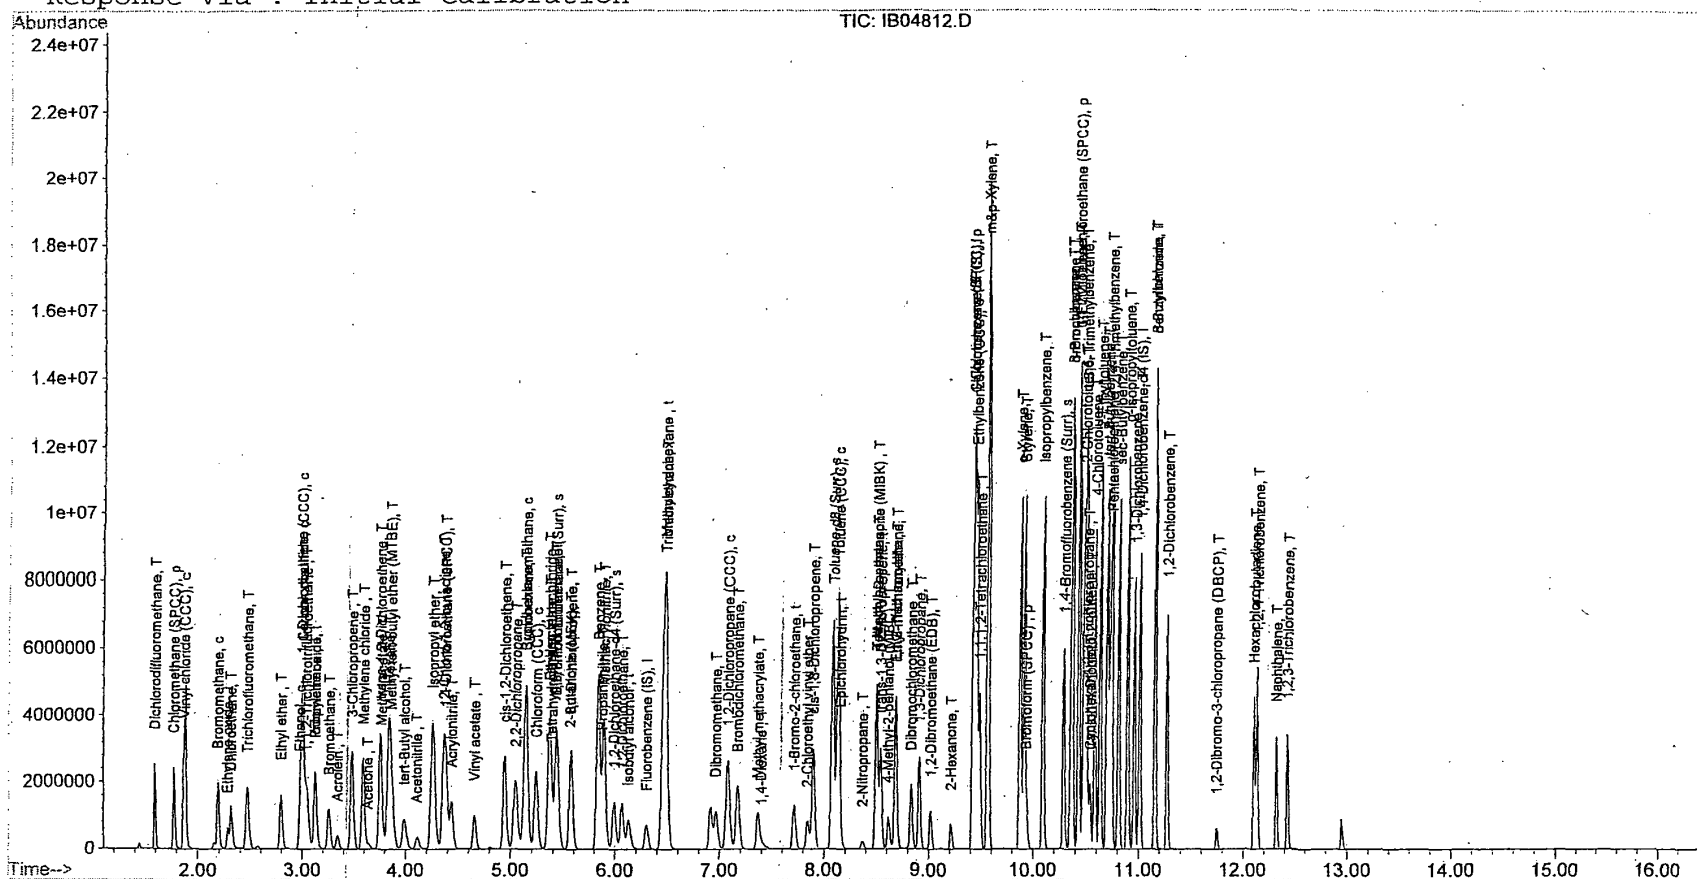

Quantitation Report (QT Reviewed)

120/132

Data File : H:\MSI.I\I110408.B\IB04819.D
 Acq On : 5 Nov 2008 5:26 pm
 Sample : 50ppb ICV; composite mix, COMP
 Misc : 1,1, 12.5uL/50mL 08MSV0816
 MS Integration Params: VOA.P
 Quant Time: Nov 7 16:00 19108

Vial: 19
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Handwritten: 11/7/08

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Fri Nov 07 15:06:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Only worked up:
 Target Analytes

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	806466	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	179195	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.01	152	239439	16.7000	PPB	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) Dibromofluoromethane (Surr)	5.43	113	202756	17.2372	PPB	0.00
Spiked Amount	16.700		Recovery	=	103.23%	
50) 1,2-Dichloroethane-d4 (Sur)	6.00	67	101919	15.1867	PPB	0.00
Spiked Amount	16.700		Recovery	=	90.96%	
64) Toluene-d8 (Surr)	8.09	98	800223	17.2821	PPB	0.00
Spiked Amount	16.700		Recovery	=	103.47%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	262347	15.6624	PPB	0.00
Spiked Amount	16.700		Recovery	=	93.77%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.59	85	778134	43.6610	PPB	S 99
3) Chloromethane (SPCC)	1.78	50	644832	36.8995	PPB	S 100
4) Vinyl chloride (CCC)	1.86	62	843039	44.6218	PPB	S 100
5) Bromomethane	2.19	94	486268	49.3563	PPB	S 99
7) Chloroethane	2.32	64	574446	45.0095	PPB	S 100
8) Trichlorofluoromethane	2.47	101	919597	46.9673	PPB	S 99
9) Ethyl ether	2.79	59	482951	48.1699	PPB	99
10) Ethanol	2.97	45	95064	1381.2115	PPB	76
11) 1,1-Dichloroethene (CCC)	2.99	96	583888	48.2760	PPB	98
12) Carbon disulfide	3.01	76	2096117	49.2708	PPB	99
13) 1,1,2-Trichlorotrifluoroet	3.04	101	507919	43.5516	PPB	98
15) Iodomethane	3.13	142	938525	50.6563	PPB	99
16) Bromoethane	3.26	108	457696	46.6182	PPB	99
18) 3-Chloropropene	3.48	41	1117385	45.5753	PPB	98
19) Methylene chloride	3.59	84	669194	48.4354	PPB	98
20) Acetone	3.64	58	33552	56.2419	PPB	91
21) trans-1,2-Dichloroethene	3.75	96	680602	50.1510	PPB	98
23) Hexane	3.84	86	218738	48.3330	PPB	# 86
24) Methyl tert-butyl ether (M	3.86	73	1429654	50.7055	PPB	80
25) tert-Butyl alcohol	3.99	59	633199	1155.7514	PPB	94
26) Acetonitrile	4.11	40	122676	251.6181	PPB	99
27) Isopropyl ether	4.26	45	2398705	48.1228	PPB	99
28) 2-Chloro-1,3-butadiene	4.36	88	126878	12.1307	PPB	99
29) 1,1-Dichloroethane (SPCC)	4.38	63	1274715	47.9396	PPB	100
30) Acrylonitrile	4.44	53	667707	263.3640	PPB	99
32) cis-1,2-Dichloroethene	4.95	96	732575	51.2175	PPB	98
33) 2,2-Dichloropropane	5.05	77	987537	49.5274	PPB	97
34) Cyclohexane	5.14	56	1192446	48.1540	PPB	100
35) Bromochloromethane	5.15	130	356717	53.2498	PPB	98
37) Chloroform (CC)	5.24	83	1153469	50.2392	PPB	99
38) Carbon tetrachloride	5.37	117	767334	49.4070	PPB	99
40) Ethyl acetate	5.37	43	1734137	270.1849	PPB	99
41) Tetrahydrofuran	5.40	72	51189	55.1221	PPB	98
43) 1,1,1-Trichloroethane	5.44	97	952738	49.6209	PPB	98

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04819.D I81104W.M Fri Nov 07 16:08:25 2008 RPT1

Data File : H:\MSI.I\I110408.B\IB04819.D
 Acq On : 5 Nov 2008 5:26 pm
 Sample : 50ppb ICV;composite mix,COMP
 Misc : 1,1, 12.5uL/50mL 08MSV0816
 MS Integration Params: VOA.P
 Quant Time: Nov 7 16:00 19108

Vial: 19
 Operator: kma
 Inst : MSI
 Multiplr: 1.00

Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Fri Nov 07 15:06:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
44) 1,1-Dichloropropene	5.58	75	905004	49.0358	PPB	97
45) 2-Butanone (MEK)	5.56	43	154997	53.0926	PPB	84
46) Benzene	5.84	78	2873143	49.4078	PPB	96
48) Propanenitrile	5.88	54	256223	268.8863	PPB	93
49) Methacrylonitrile	5.90	67	146802	47.9236	PPB #	88
51) 1,2-Dichloroethane	6.07	62	660290	47.0630	PPB	99
52) Isobutyl alcohol	6.13	43	302188	1031.4614	PPB	100
54) Trichloroethene	6.50	130	658158	48.8338	PPB	98
55) Dibromomethane	6.97	93	267322	52.8215	PPB	99
56) n-Butanol	6.92	56	500393	2582.2918	PPB	98
57) 1,2-Dichloropropane (CCC)	7.08	63	687267	50.5172	PPB	99
58) Bromodichloromethane	7.17	83	781174	50.0544	PPB	99
59) 1,4-Dioxane	7.41	88	72146	1188.1733	PPB	93
60) Methyl methacrylate	7.37	69	263380	47.4179	PPB	98
61) i-Bromo-2-chloroethane	7.71	63	719235	50.0416	PPB	99
62) cis-1,3-Dichloropropene	7.90	75	1021055	53.1049	PPB	97
66) Toluene (CCC)	8.13	91	2818030	46.5831	PPB	99
67) Epichlorohydrin	8.16	57	144924	235.0352	PPB	81
68) 2-Nitropropane	8.37	43	312766	205.8607	PPB #	66
69) Tetrachloroethene	8.51	164	491265	49.0707	PPB	99
70) 4-Methyl-2-pentanone (MIBK)	8.51	43	335172	54.9419	PPB	98
71) trans-1,3-Dichloropropene	8.55	75	823011	52.8088	PPB	98
72) 1,1,2-Trichloroethane	8.69	97	408980	49.5858	PPB	98
73) 4-Methyl-2-pentanol (MIBC)	8.62	45	59692	50.1365	PPB	96
74) Ethyl methacrylate	8.69	69	546917	47.5416	PPB	98
75) Dibromochloromethane	8.83	129	487557	54.8075	PPB	100
76) 1,3-Dichloropropane	8.91	76	828677	49.4574	PPB	99
77) 1,2-Dibromoethane (EDB)	9.02	107	381032	52.2543	PPB	99
78) 2-Hexanone	9.22	43	223066	59.4920	PPB	99
79) Chlorobenzene (SPCC)	9.44	112	1814028	48.6603	PPB	98
80) 1-Chlorohexane	9.42	55	628431	48.1911	PPB	99
81) Ethylbenzene (CCC)	9.46	106	1014767	48.0061	PPB	92
82) 1,1,1,2-Tetrachloroethane	9.49	131	586339	51.3872	PPB	100
83) m&p-Xylene	9.57	106	2561829	97.8012	PPB	98
84) o-Xylene	9.88	106	1205863	49.6839	PPB	99
85) Bromoform (SPCC)	9.94	173	240900	60.5762	PPB	100
86) Styrene	9.92	104	1849201	51.4395	PPB	99
87) Isopropylbenzene	10.09	105	2944035	51.4710	PPB	100
88) Bromobenzene	10.36	156	636613	52.3151	PPB	99
89) n-Propylbenzene	10.37	120	825148	50.9023	PPB	99
90) 1,1,2,2-Tetrachloroethane	10.43	83	426419	49.8632	PPB	99
93) 2-Chlorotoluene	10.48	126	683627	49.1529	PPB	98
94) Cyclohexanone	10.54	42	518090	3715.2111	PPB	94
95) 1,2,3-Trichloropropane	10.52	110	137911	48.0542	PPB	90
96) trans-1,4-Dichloro-2-buten	10.54	53	97619	45.9322	PPB	79
97) 3-Ethyltoluene	10.43	105	2839061	47.9593	PPB	100
98) 4-Chlorotoluene	10.59	126	702236	50.9277	PPB	99
99) 1,3,5-Trimethylbenzene	10.50	105	2380964	47.6262	PPB	65
100) 2-Ethyltoluene	10.64	105	2861430	47.6871	PPB	77

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 TR04819.D I81104W.M Fri Nov 07 16:08:26 2008 RPT1

Quantitation Report (QT Reviewed)

122/132

Data File : H:\MSI.I\I110408.B\IB04819.D Vial: 19
 Acq On : 5 Nov 2008 5:26 pm Operator: kma
 Sample : 50ppb ICV;composite mix,COMP Inst : MSI
 Misc : 1,1, 12.5uL/50mL 08MSV0816 Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Nov 7 16:00 19108 Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Fri Nov 07 15:06:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
101) tert-Butylbenzene	10.70	91	1291260	47.0593	PPB	# 73
102) Pentachloroethane	10.73	167	377205	54.0155	PPB	99
103) 1,2,4-Trimethylbenzene	10.75	105	2386955	47.6795	PPB	99
104) sec-Butylbenzene	10.82	105	3012398	49.3302	PPB	99
105) p-Isopropyltoluene	10.90	119	2594816	49.7191	PPB	99
106) 1,3-Dichlorobenzene	10.96	146	1223421	49.3817	PPB	100
107) 1,4-Dichlorobenzene	11.02	146	1229594	46.8814	PPB	99
108) Benzyl chloride	11.16	126	156394	44.0303	PPB	91
109) n-Butylbenzene	11.16	134	632698	51.9323	PPB	93
110) 1,2-Dichlorobenzene	11.27	146	1032592	50.1131	PPB	100
112) 1,2-Dibromo-3-chloropropan	11.75	157	64899	54.2404	PPB	# 1
113) Hexachlorobutadiene	12.11	225	281880	45.0881	PPB	99
114) 1,2,4-Trichlorobenzene	12.14	180	589552	53.5776	PPB	99
115) Naphthalene	12.33	128	895267	55.9515	PPB	100
116) 1,2,3-Trichlorobenzene	12.44	180	392316	50.2082	PPB	99

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04819.D I81104W.M Fri Nov 07 16:08:26 2008 RPT1


Quantitation Report

Data File : C:\HPCHEM\1\DATA\I110408.B\IB04819.D
Acq On : 5 Nov 2008 5:26 pm
Sample : 50ppb ICV; composite mix
Misc : 1,1, 12.5uL/50mL 08MSV0816
MS Integration Params: VOA.P
Quant Time: Nov 5 17:42 19108

Vial: 19
Operator: kma
Inst : MSI
Multiplr: 1.00


Quant Results File: I81104W.RES

Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Wed Nov 05 13:16:55 2008
Response via : Initial Calibration

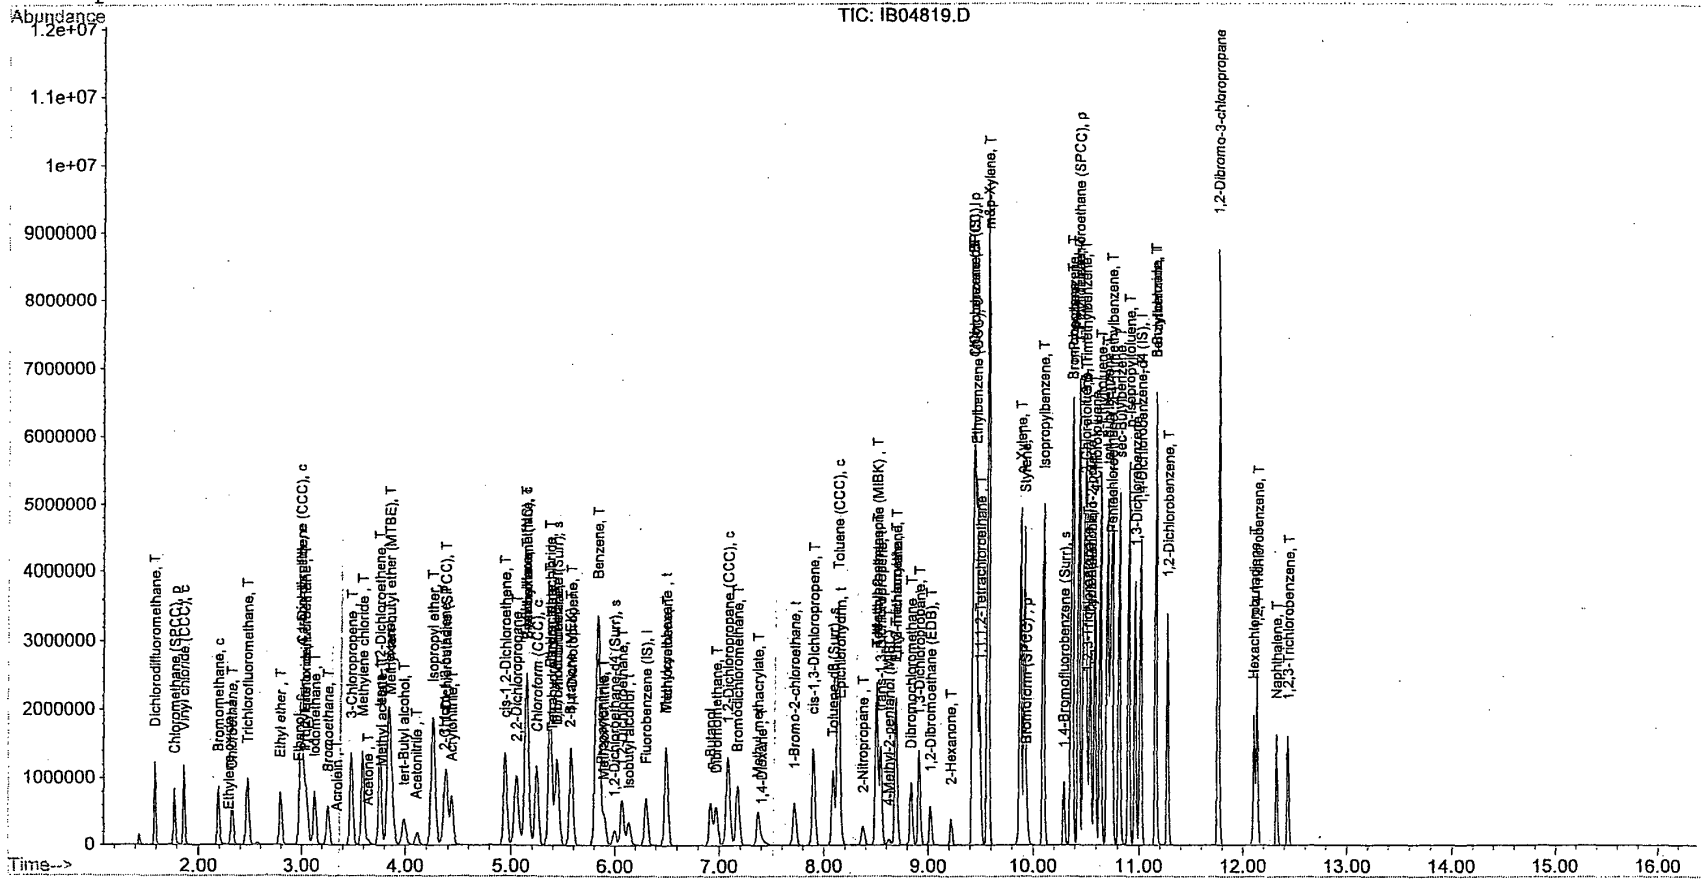

BFB

Data File : H:\MSI.I\I110408.B\IB04819.D Vial: 19
 Acq On : 5 Nov 2008 5:26 pm Operator: kma
 Sample : 50ppb ICV; composite mix, COMP Inst : MSI
 Misc : 1,1, 12.5uL/50mL 08MSV0816 Multiplr: 1.00
 MS Integration Params: VOA.P
 Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water

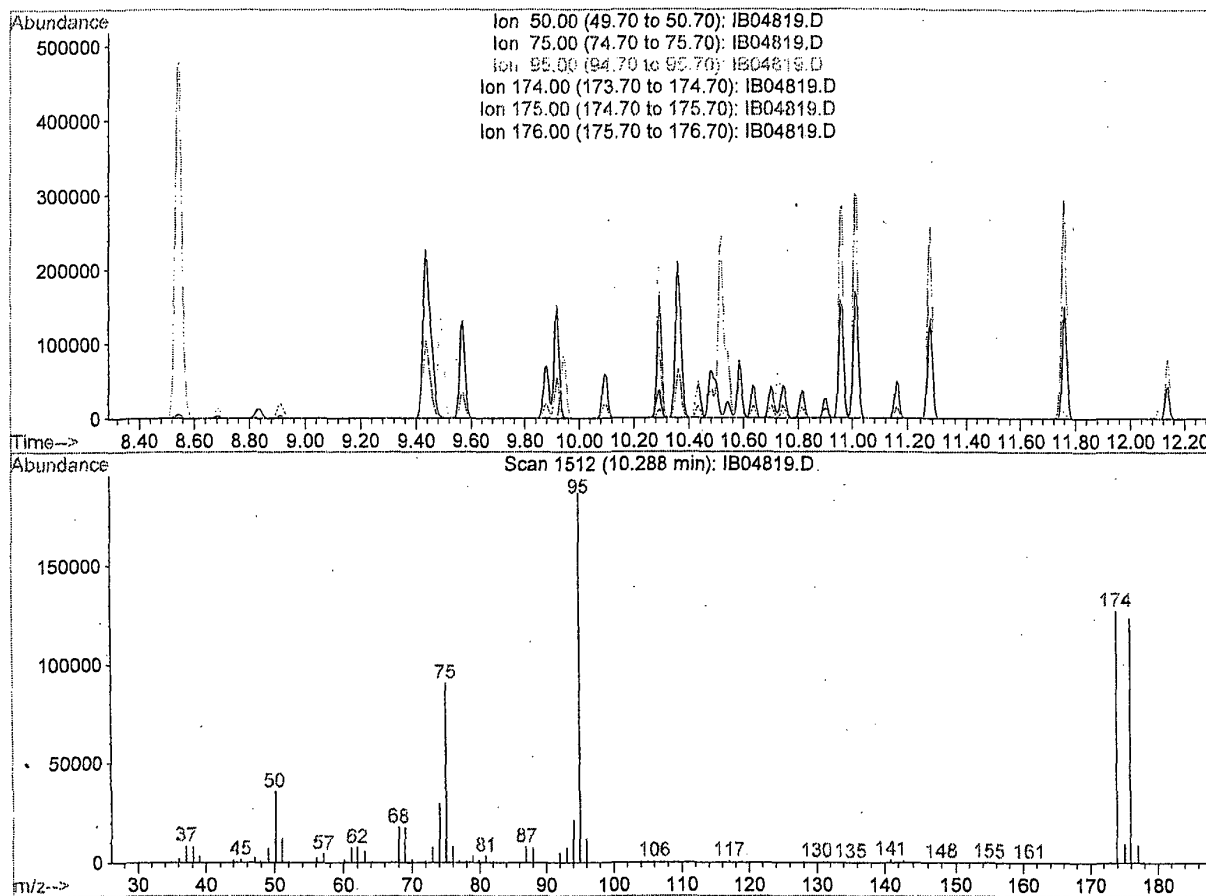

Spectrum Information: Scan 1512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	35792	PASS
75	95	30	60	48.7	90568	PASS
95	95	100	100	100.0	186112	PASS
96	95	5	9	6.4	11993	PASS
173	174	0.00	2	0.6	706	PASS
174	95	50	100	68.4	127384	PASS
175	174	5	9	7.2	9214	PASS
176	174	95	101	97.1	123672	PASS
177	176	5	9	7.2	8847	PASS

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04822.D Vial: 22
 Acq On : 6 Nov 2008 11:43 am Operator: kma
 Sample : 50ppb ICV;reactives mix,RC Inst : MSI
 Misc : 1,1, 12.5/50 08MSV0819/810 25/50 08MSV08 Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Nov 7 16:02 19108 Quant Results File: I81104W.RES

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Fri Nov 07 15:06:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Only worked up:
 Target Analytes

Good 11/7/08
2-came only Remn Acrolein/VA due to incorrect prep.


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.30	96	814251	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	164213	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.00	152	212949	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	192185	16.1823	PPB	0.00
Spiked Amount	16.700		Recovery	=	96.89%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	94826	13.9947	PPB	0.00
Spiked Amount	16.700		Recovery	=	83.77%	
64) Toluene-d8 (Surr)	8.08	98	793474	16.9725	PPB	0.00
Spiked Amount	16.700		Recovery	=	101.62%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	251537	16.3871	PPB	0.00
Spiked Amount	16.700		Recovery	=	98.14%	
Target Compounds						
17) Acrolein	3.33	56	326245	466.3598	PPB	100
31) Vinyl acetate	4.65	43	2141674	131.8808	PPB	99
63) 2-Chloroethyl vinyl ether	7.84	63	241611	59.0747	PPB	97

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 TR04822.D I81104W.M Fri Nov 07 16:08:37 2008 RPT1

Quantitation Report

Data File : C:\HPCHEM\1\DATA\I110408.B\IB04822.D Vial: 22
Acq On : 6 Nov 2008 11:43 am Operator: kma
Sample : 50ppb ICV;reactives mix Inst : MSI
Misc : 1,1, 12.5/50 08MSV0819/810 25/50 08MSV08 Multiplr: 1.00
MS Integration Params: VOA.P
Quant Time: Nov 6 12:00 19108 Quant Results File: I81104W.RES

Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Wed Nov 05 13:16:55 2008
Response via : Initial Calibration

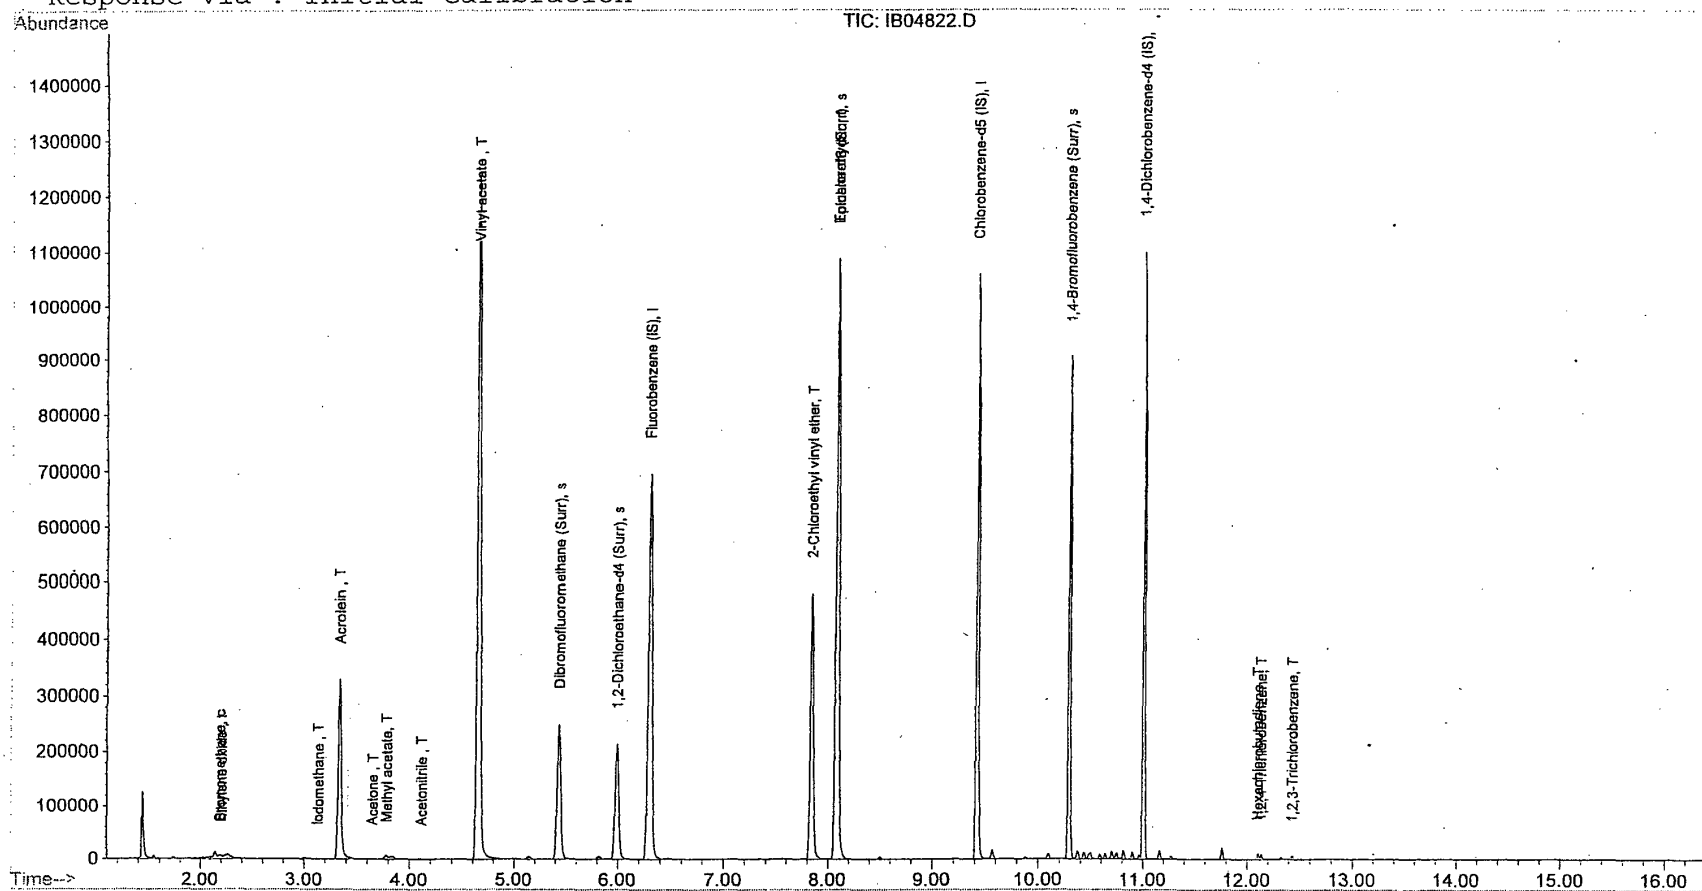

Quantitation Report (QT Reviewed)

Data File : H:\MSI.I\I110408.B\IB04825.D Vial: 25
 Acq On : 6 Nov 2008 3:39 pm Operator: kma
 Sample : 50ppb ICV;MIX 5 10X ICV,MIX5 Inst : MSI
 Misc : 1,1, 12.5uL/50mL 08MSV0822 Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Nov 7 16:04 19108 Quant Results File: I81104W.RES

2007
11/7/08

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Fri Nov 07 15:06:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	817572	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	165279	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.00	152	217260	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	191906	16.0932	PPB	0.00
Spiked Amount	16.700		Recovery	=	96.35%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	97008	14.2586	PPB	0.00
Spiked Amount	16.700		Recovery	=	85.39%	
64) Toluene-d8 (Surr)	8.08	98	769893	16.4012	PPB	0.00
Spiked Amount	16.700		Recovery	=	98.20%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	247119	15.9955	PPB	0.00
Spiked Amount	16.700		Recovery	=	95.81%	
Target Compounds						
					Qvalue	
9) Ethyl ether	2.79	59	449248	44.1996	PPB	99
13) 1,1,2-Trichlorotrifluoroet	3.04	101	468844	39.6550	PPB	99
18) 3-Chloropropene	3.48	41	1066793	42.9207	PPB	98
24) Methyl tert-butyl ether (M)	3.86	73	1307188	45.7322	PPB	# 22
25) tert-Butyl alcohol	3.98	59	518285	933.1531	PPB	93
26) Acetonitrile	4.10	40	110033	222.6206	PPB	96
30) Acrylonitrile	4.43	53	607749	236.4585	PPB	99
41) Tetrahydrofuran	5.40	72	36574	38.8492	PPB	# 43
48) Propanenitrile	5.87	54	225370	233.2957	PPB	92
49) Methacrylonitrile	5.89	67	132242	42.5840	PPB	90
52) Isobutyl alcohol	6.12	43	244026	825.6688	PPB	99
59) 1,4-Dioxane	7.41	88	57781	938.6694	PPB	92
60) Methyl methacrylate	7.37	69	229119	40.7970	PPB	97
68) 2-Nitropropane	8.36	43	153292	109.3910	PPB	100
74) Ethyl methacrylate	8.69	69	473519	44.6499	PPB	99
94) Cyclohexanone	10.54	42	562577	4446.0605	PPB	95
96) trans-1,4-Dichloro-2-buten	10.54	53	86988	45.1083	PPB	73

(#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 I81104W.M Fri Nov 07 16:08:59 2008 RPT1

Quantitation Report

Data File : C:\HPCHEM\1\DATA\I110408.B\IB04825.D Vial: 25
 Acq On : 6 Nov 2008 3:39 pm Operator: kma
 Sample : 50ppb ICV;MIX 5 10X ICV Inst : MSI
 Misc : 1,1, 12.5uL/50mL 08MSV0822 Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Nov 6 15:56 19108 Quant Results File: I81104W.RES

Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Nov 05 13:16:55 2008
 Response via : Initial Calibration

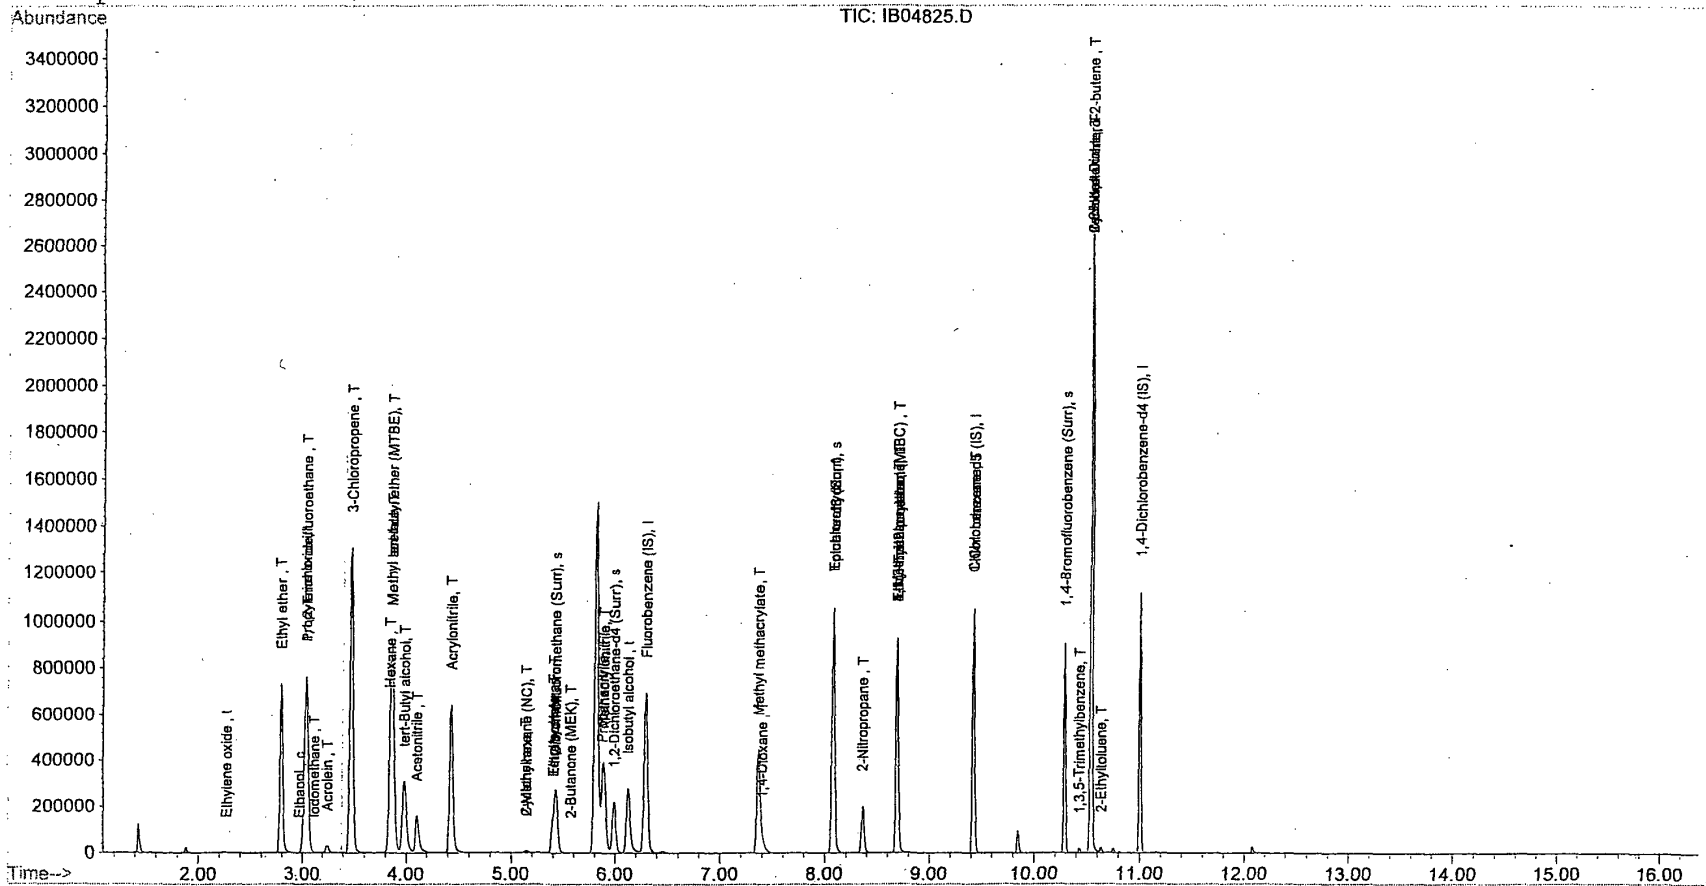

Data File : H:\MSI.I\I110408.B\IB04826.D Vial: 26
 Acq On : 6 Nov 2008 4:07 pm Operator: kma
 Sample : 50ppb ICV;special analytes mix,SPECIAL Inst : MSI
 Misc : 1,1, 12.5uL/50mL 08MSV0821 Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Nov 7 16:06 19108 Quant Results File: I81104W.RES

*Zoom
11/7/08*

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Fri Nov 07 15:06:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.30	96	820088	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	175578	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.00	152	221747	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.43	113	196439	16.4228	PPB	0.00
Spiked Amount	16.700		Recovery	=	98.32%	
50) 1,2-Dichloroethane-d4 (Sur)	5.99	67	104041	15.2454	PPB	0.00
Spiked Amount	16.700		Recovery	=	91.32%	
64) Toluene-d8 (Surr)	8.08	98	783743	16.6450	PPB	0.00
Spiked Amount	16.700		Recovery	=	99.70%	
91) 1,4-Bromofluorobenzene (Su)	10.29	95	248969	15.1699	PPB	0.00
Spiked Amount	16.700		Recovery	=	90.84%	
Target Compounds						
6) Ethylene oxide	2.29	44	728220	497.7105	PPB	99
14) Propylene oxide	3.12	58	342026	235.6408	PPB	98
22) Methyl acetate	3.77	74	126118	119.8765	PPB	98
53) Methylcyclohexane	6.47	83	2053547	115.5646	PPB	99
68) 2-Nitropropane	8.36	43	71808	48.2372	PPB	99
94) Cyclohexanone	10.54	42	35261	273.0298	PPB	96

 (#)=qualifier out of range (m)=manual integration (S)=analyte in sublist
 IB04826.D I81104W.M Fri Nov 07 16:09:10 2008 RPT1

Quantitation Report

Data File : C:\HPCHEM\1\DATA\I110408.B\IB04826.D Vial: 26
 Acq On : 6 Nov 2008 4:07 pm Operator: kma
 Sample : 50ppb ICV;special analytes mix Inst : MSI
 Misc : 1,1, 12.5uL/50mL 08MSV0821 Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Nov 6 16:24 19108 Quant Results File: I81104W.RES

Method : C:\HPCHEM\1\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Wed Nov 05 13:16:55 2008
 Response via : Initial Calibration

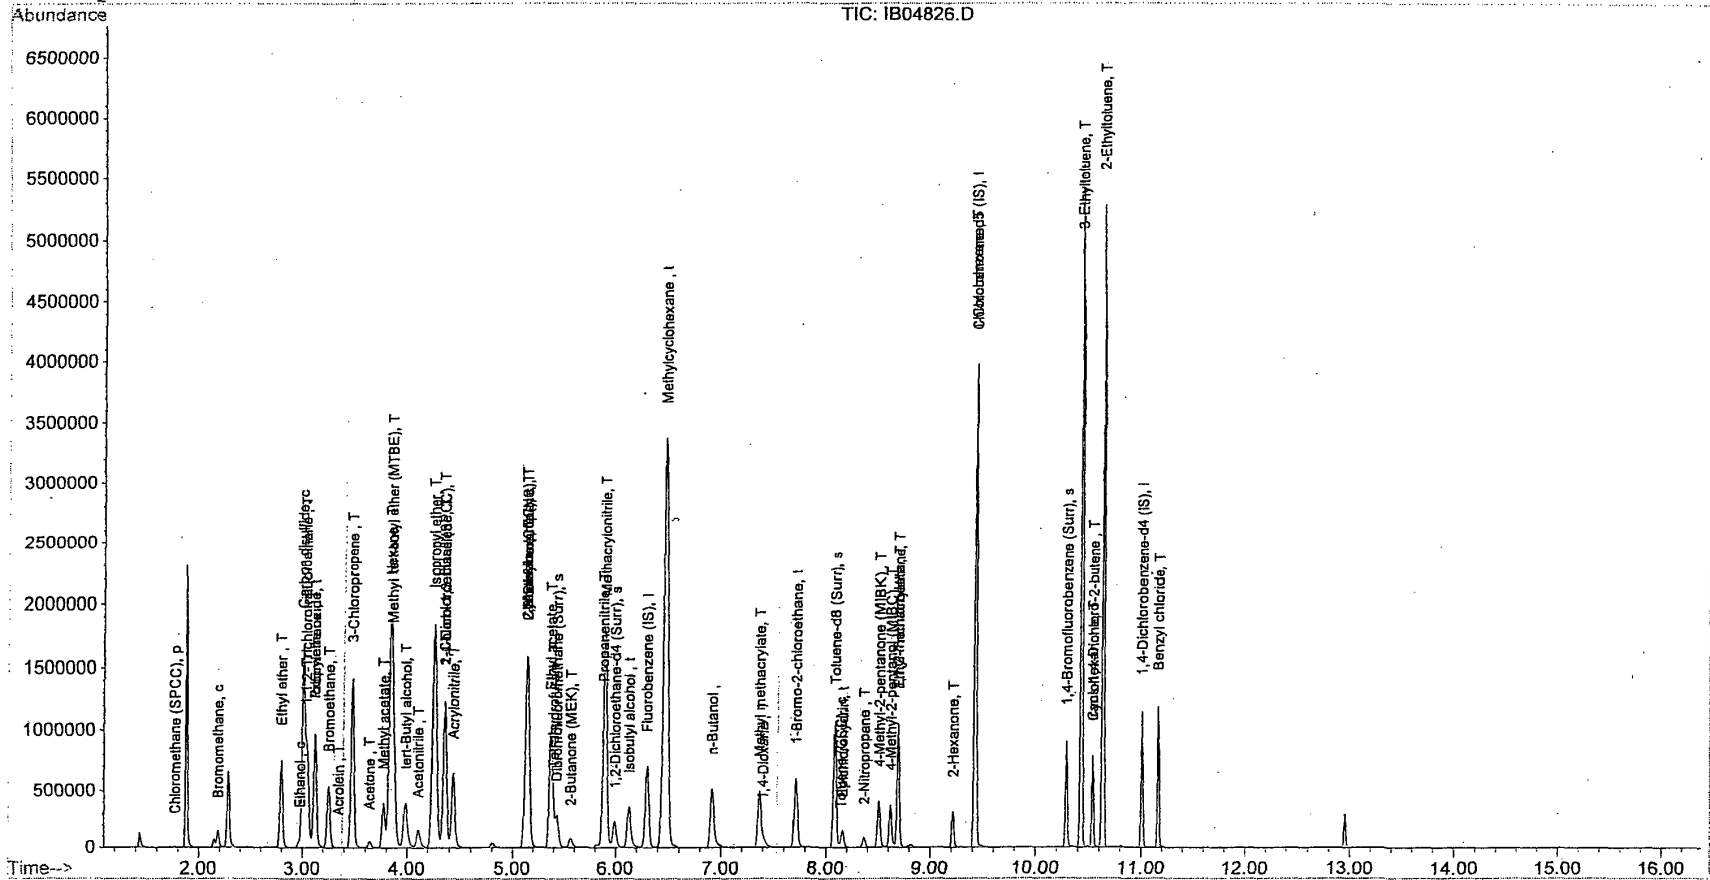

Data File : H:\MSI.I\I110408.B\IB04827.D Vial: 27
 Acq On : 7 Nov 2008 7:54 am Operator: dy
 Sample : 50ppb ICV;acrolein ICV 10x,RC Inst : MSI
 Misc : 1,1, 12.5uL/50mL 08MSV0824 Multiplr: 1.00
 MS Integration Params: VOA.P
 Quant Time: Nov 7 16:07 19108 Quant Results File: I81104W.RES

Don
11/7/08

Quant Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
 Title : EPA Method 8260B/624 Calibration Curve 15mL Water
 Last Update : Fri Nov 07 15:06:06 2008
 Response via : Initial Calibration
 DataAcq Meth : I81104W

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.29	96	813861	16.7000	PPB	0.00
65) Chlorobenzene-d5 (IS)	9.42	119	164262	16.7000	PPB	0.00
92) 1,4-Dichlorobenzene-d4 (IS)	11.00	152	210069	16.7000	PPB	0.00
System Monitoring Compounds						
42) Dibromofluoromethane (Surr)	5.42	113	191667	16.1464	PPB	0.00
Spiked Amount	16.700		Recovery	=	96.71%	
50) 1,2-Dichloroethane-d4 (Sur)	5.98	67	93803	13.8504	PPB	0.00
Spiked Amount	16.700		Recovery	=	82.93%	
64) Toluene-d8 (Surr)	8.08	98	792589	16.9617	PPB	0.00
Spiked Amount	16.700		Recovery	=	101.56%	
91) 1,4-Bromofluorobenzene (Su)	10:29	95	252065	16.4166	PPB	0.00
Spiked Amount	16.700		Recovery	=	98.32%	
Target Compounds						
17) Acrolein	3.33	56	130396	186.4874	PPB	99

Quantitation Report

Data File : C:\HPCHEM\1\DATA\I110408.B\IB04827.D Vial: 27
Acq On : 7 Nov 2008 7:54 am Operator: dy
Sample : 50ppb ICV;acrolein ICV 10x Inst : MSI
Misc : 1,1, 12.5uL/50mL 08MSV0824 Multiplr: 1.00
Quant Time: Nov 7 8:23 19108 Quant Results File: I81104W.RES

Method : H:\MSI.I\METHODS\I81104W.M (RTE Integrator)
Title : EPA Method 8260B/624 Calibration Curve 15mL Water
Last Update : Thu Nov 06 14:17:10 2008
Response via : Initial Calibration

